

Instructions for use / installation of the boso profil-manager XD

Powerful software for computer-assisted
blood pressure control and observation of therapy



Compatible with the following blood pressure meters:

TM-2430
ABI-system 100
ABI-system 100 PWV
medicus PC2
medilife PC3

These instructions for use and installation of the boso profil-manager XD apply to version 4.2.0.128 and above. Please refer to the readme.txt file on the installation CD for new information.

The drive letters in these instructions for use are simply examples:

C:\ for the local hard drive

D:\ for the CD/DVD drive

The path data corresponds to a standard single-user installation under the german Windows 7 (32-bit) operating system and may be different in other operating systems or language versions.

Table of contents

1.1	Before installation.....	7
1.1.1	Data backup.....	7
1.1.2	Operating the software	7
1.2	Installing boso profil-manager XD	8
1.2.1	Single-user version.....	9
1.2.2	Networkversion	12
1.2.2.1	Installing the Firebird database server.....	12
1.2.2.2	Installing the database file	13
1.2.2.3	Installing boso profil-manager XD.....	13
1.2.2.4	Launching the network version for the first time	14
1.3	Converting data from profilmanager 3 and ABI.....	15
1.4	Installing the USB connection cable.....	17
2.	Start	18
2.1	Patient registry, for all applications.....	19
2.1.1	„New...“ button	19
2.1.2	„Modify...“ button	19
2.1.3	„Delete...“ button	19
2.1.4	„Export/Import“ button.....	19
2.1.4.1	„Export Excel“	19
2.1.4.2	„Export patient (XML)“	19
2.1.4.3	„Import patient (XML)“	20
2.1.5	„Import GDT“	20
2.1.6	„Settings...“ button	20
2.1.7	„Print...“ button	20
2.1.8	„Billing assistance“ button	21
3.	„ABI/PWV measurement“ application.....	22
3.1	„Patient“ registry	22
3.2	„Measurements“ registry.....	22
3.2.1	„Delete“ button	23
3.2.2	„Export GDT“ button	23
3.2.3	„Remarks...“ button	24
3.2.4	„Print“ button.....	24
3.2.5	„ABI measurement“ button.....	25
3.2.6	„ABI+PWV measurement“ button	25
3.3	„Profiles“ registry	26
3.3.1	„Print“ button	27
3.4	„Settings...“ button in „Patient“ registry	28
3.4.1	„Doctor“ sub-registry	28
3.4.2	„Import/Export“ sub-registry.....	29
3.4.3	„Classification“ sub-registry.....	30
3.4.4	„Test mode“ sub-registry	31
3.4.5	„Printer settings“ sub-registry.....	32
3.4.6	Error-codes	32

4.	„24-hour measurement“ application.....	33
4.1	„Patient“ registry	33
4.2	„Measurements“ registry.....	33
4.2.1	„Delete period“ button	36
4.2.2	„Export GDT“ button	36
4.2.3	„Manual data“ button	36
4.2.4	„Print...“ button.....	36
4.2.5	„Initialise“ button.....	37
4.2.6	„Trasfer data“ button.....	39
4.3	„Sys/dia profile“ registry	40
4.3.1	„Modify“ button	40
4.3.2	„Reference chart“ button	40
4.3.3	„Time scope“ selection field	41
4.3.4	„Print...“ button	41
4.4	„MAP profile“ registry	42
4.4.1	„Modify“ button	42
4.4.2	„Reference chart“ selection field	42
4.4.3	„Time scope“ selection field	43
4.4.4	„Print...“ button	43
4.5	„Profil PP profile“ registry	44
4.5.1	„Modify“ button	44
4.5.2	„Reference chart“ selection field	45
4.5.3	„Time scope“ selection field	45
4.5.4	„Print...“ button	45
4.6	„Statistics“ button.....	46
4.6.1	„Modify“ button	47
4.6.2	„Print...“ button	47
4.7	„Settings...“ button in „Patient“ registry	48
4.7.1	„Doctor“ sub-registry	48
4.7.2	„Import/export“ sub-registry.....	49
4.7.3	„Printer settings“ sub-registry.....	50
4.7.4	„Interface“ sub-registry	51
4.7.5	„Limits“ sub-registry.....	52
4.7.6	„Profile“ sub-registry.....	53
5.	„Patient measurement“ application.....	54
5.1	„Patient“ registry	54
5.2	„Measurements“ registr	54
5.2.1	„Delete period“ button	56
5.2.2	„Export GDT“ button	56
5.2.3	„Manual data“ button	56
5.2.4	„Print...“ button.....	56
5.2.5	„Trasfer data“ button.....	57
5.2.6	„Interval limits“ button.....	58
5.2.7	„All, Morning, Afternoon“ selection.....	58
5.2.8	„Period“ selection	58

5.3	„Sys/dia profile“ registry	59
5.3.1	„All, Morning, Afternoon“ selection	59
5.3.2	„Period“ selection	60
5.3.3	„Time scope“ selection field	60
5.3.4	„Print...“ button	60
5.4	„MAP profile“ registry	61
5.4.1	„All, Morning, Afternoon“ selection	61
5.4.2	„Period“ selection	62
5.4.3	„Time scope“ selection field	62
5.4.4	Print...“ button	62
5.5	„PP profile“ registry	63
5.5.1	„All, Morning, Afternoon“ selection	63
5.5.2	„Time scope“ selection field	64
5.5.3	„Period“ selection	64
5.5.4	„Print...“ button	64
5.6	„Statistics“ button	65
5.6.1	„Print...“ button	66
5.7	„Settings...“ button in „Patient“ registry	67
5.7.1	„Doctor“ sub-registry	67
5.7.2	„Import/export“ sub-registry	68
5.7.3	„Printer settings“ sub-registry	69
5.7.4	„Interface“ sub-registry	70
5.7.5	„Limits“ sub-registry	71
5.7.6	„Profile“ sub-registry	72
6.	Warranty provisions	73
7.	Limitation of liability	74
8.	Explanation of symbols	74
Appendix A – Extract from GDT record description		75

Contents of package

1 installation CD

1 user manual

Minimum operating requirements:

- Pentium II or higher
- 512 MB RAM
- Graphics card
- 100 MB free hard disk space
- USB 1.1 interface
- Microsoft Windows® XP

Purpose

software, utilized for

- management of values which are generated by measuring instruments
- archive of measured values in a separate database
- data exchange with doctors' EDP systems via GDT interface
- programming of 24-blood pressure instruments (interval limits, interval time, maximum inflation pressure)
- control of ABI measurement systems (start and termination of a measurement)

1.1 Before installation...

You have chosen boso profil-manager XD, a software solution which gives you optimum results with minimum input time. It has been deliberately designed to be operated without the usual menu structure based on individual registries. This is why the user manual also refers to individual windows and program parts as registries.

1.1.1 Data backup

To avoid losing data, you should back up the 'profman.fdb' file from the C:\ProgramData\Boso\profmanXD\ sub-directory at regular intervals.

1.1.2 Operating the software

The program is operated by the mouse.



PC requirements

Computers used to assess data must comply with the latest version of European standard EN 60601-1.


1.2 Installing boso profil-manager XD

To install boso profil-manager XD, start file D:\installer.exe manually or automatically via the autostart function which runs when you have inserted the CD.



Make sure that you have administrator rights when installing the program (if in doubt, start the "installer.exe" program with the right mouse button, "execute as administrator")

The following selection screen (in German) will appear as soon as the program has started:

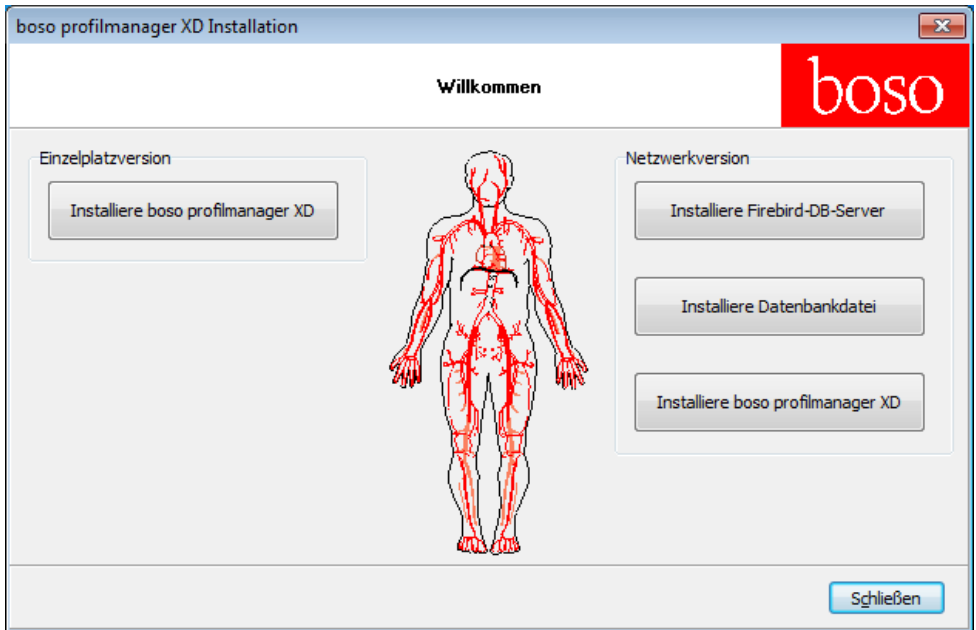


Choose either the single-user version or the network version.

1.2.1 Single-user version


The single-user version is the correct choice if you are only going to run the program on one computer. In this case you do not need to install a separate Firebird database server (an embedded Firebird is used). Follow the installation assistant instructions:

Select your preferred language for installation (screenshot in German):

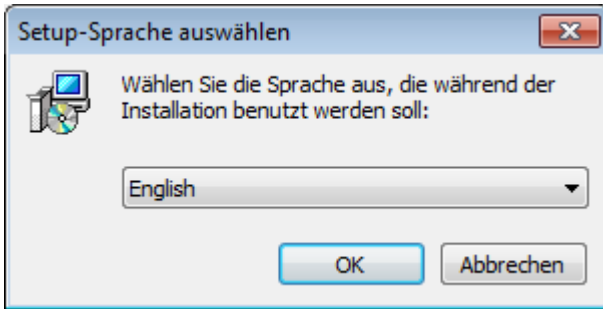


The available languages are German, English and French.


As the program can be used with all current boson PC devices, in the next mask you must select the type of device to be activated when starting the program for the first time. After installation you can switch between device types at any time while using the program.

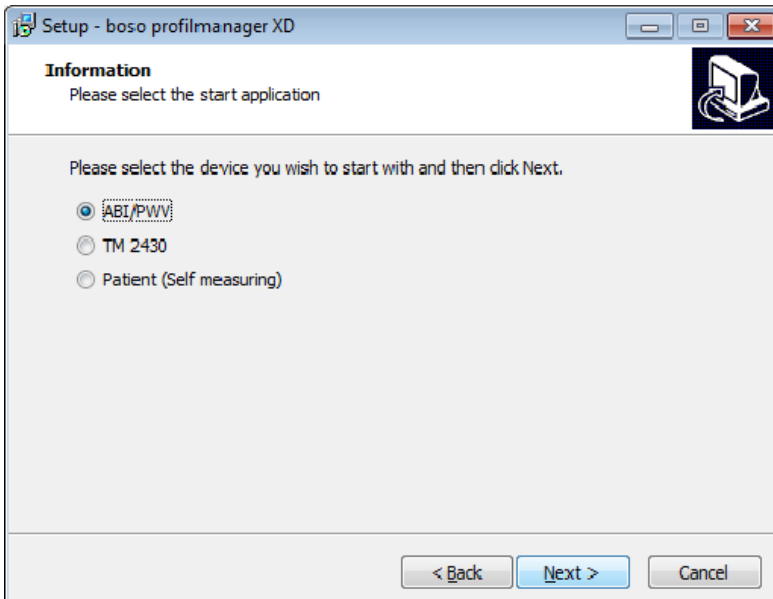

You can change the target folder for installation individually, but in most cases the default folder is used unchanged:

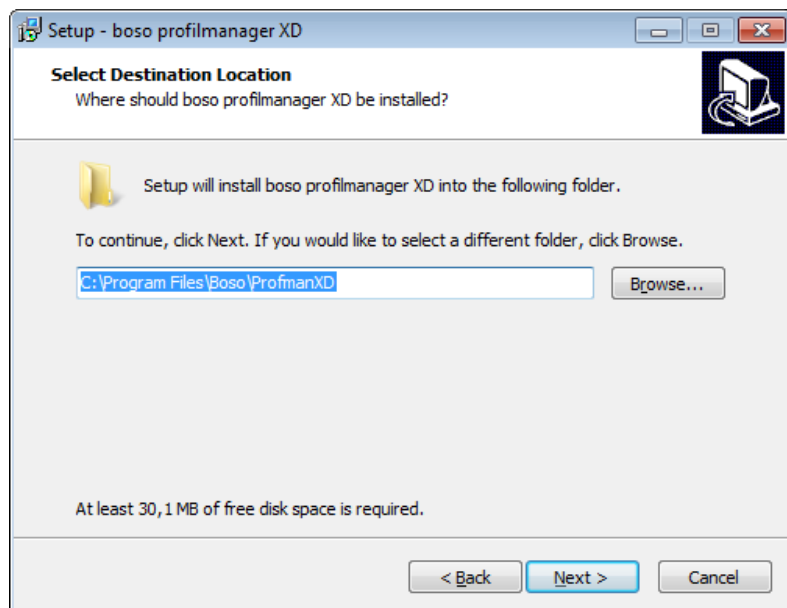


At the end of installation, tick the “Install boso USB Driver” checkbox to install the USB driver needed for the PC connection cable.

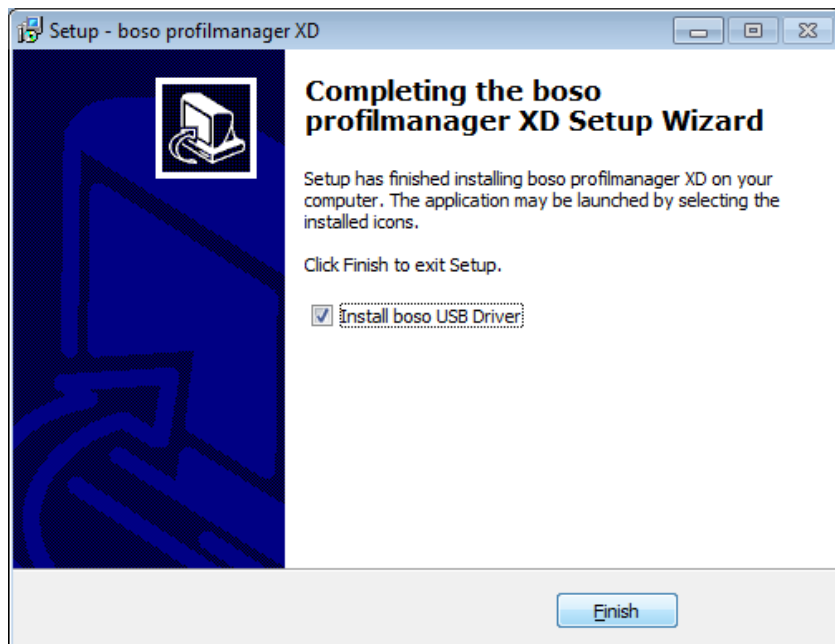

Once you have successfully installed the single-user version of boso profil-manager XD, click on the “Close” button to close the installation screen.

1.2.2 Network version (screenshot in German)

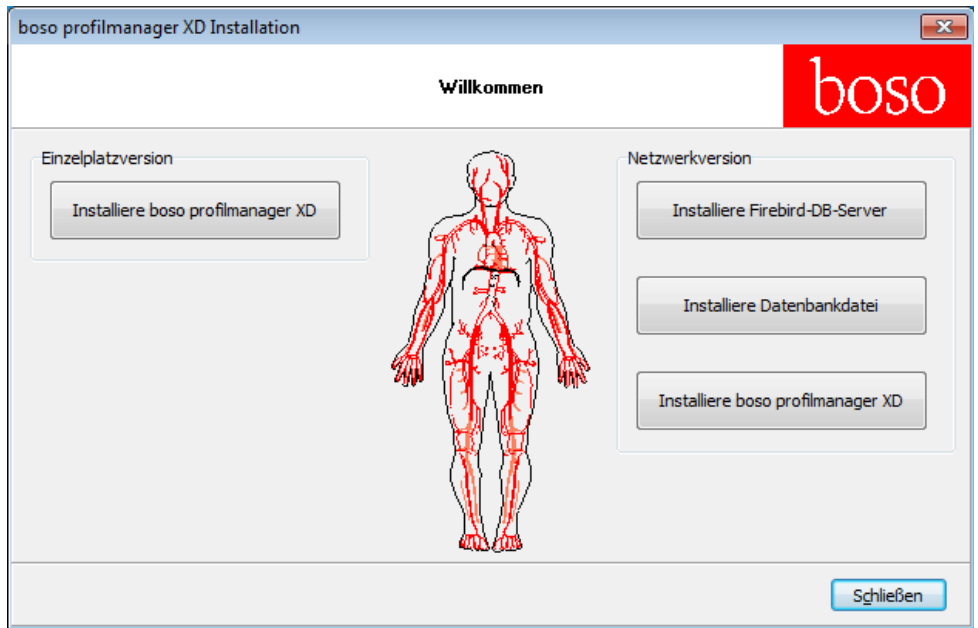

The network version is the correct choice if you are going to run the program on multiple workstations in a network. Here the database can be stored at any location in the network.

1.2.2.1 Installing the Firebird database server

In order to run the network version of boso profil-manager XD, the Firebird database server must be installed on the computer where the database is to be stored.

Click on the “Install Firebird DB server” button to install the Firebird database server.



After selecting the language, follow the instructions given by the installation assistant and accept all the default settings

1.2.2.2 Installing the database file

The “profman.fdb” database file can be stored at any location in the network.



Make sure that the computer in which the database is to be located is running a current Firebird server (version 2.5 or above), that the TCP port 3050 is open for access when the firewall is active, and that access to the database and the database server is not blocked by an anti-virus program.


1.2.2.3 Installing boso profil-manager XD

You can install boso profil-manager XD on any computer in the network by clicking the “Install boso profil-manager XD” button.

Follow the instructions given by the installation assistant as described for the [single-user version] in chapter 1.2.1.

1.2.2.4 Launching the network version for the first time

When you launch the network version for the first time, you will see a login window to register with the Firebird database.

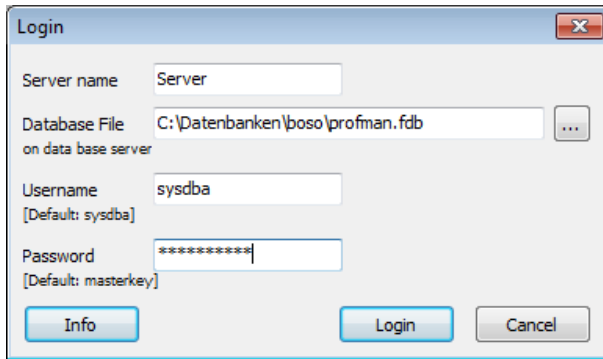A screenshot of a Windows-style dialog box titled "Login". It contains four input fields: "Server name" with the text "Server", "Database File" with the text "C:\Datenbanken\boso\profman.fdb" and a browse button "...", "Username" with the text "sysdba" and a hint "[Default: sysdba]", and "Password" with masked text "*****" and a hint "[Default: masterkey]". At the bottom are three buttons: "Info", "Login", and "Cancel".

The login data you enter here will be stored in the "profman.ini" file in the C:\Programme\Boso\ProfmanXD\ directory and can be modified if necessary at any time, for instance if the database is moved to another location in the network.

Server name

Name of the server in which the database is located

Database file



Drive, path and name of the boso profil-manager XD database file from the server's perspective.

User name

Login information for the current Firebird database server. The default name is "sysdba". Login information may be different if Firebird has already been installed.


Password

Login information for the current Firebird database server. The default password is "masterkey". Login information may be different if Firebird has already been installed.

1.3 Converting data from boso profil-manager 3 and ABI

Use the Konverter.exe program to convert existing data from earlier Firebird databases.

Launch the program either via Windows Explorer from the directory path C:\Programme\Boso\ProfmanXD\ or via the Windows start button, selecting the program “Transfer data from boso profil-manager 3” under the “boso profil-manager XD” program group (file path in German)

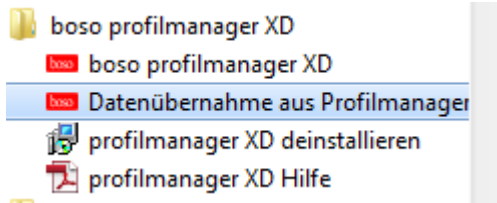


The databases to be converted must be on the local system. Conversion via the network is not possible.

Enter a username and password to register with the Firebird database server. The default username is "sysdba" and the default password is "masterkey".

Select the storage location for the profil-manager XD file in the "Target DB (profil-manager XD)" field.

Select the storage location of the database you want to convert (ABI or profil-manager 3). Click on the "Connect" button to connect to the source database.

Once you have established a connection with the source database, start transferring data by clicking on the button of the same name ("Start transfer") (screenshot in German).

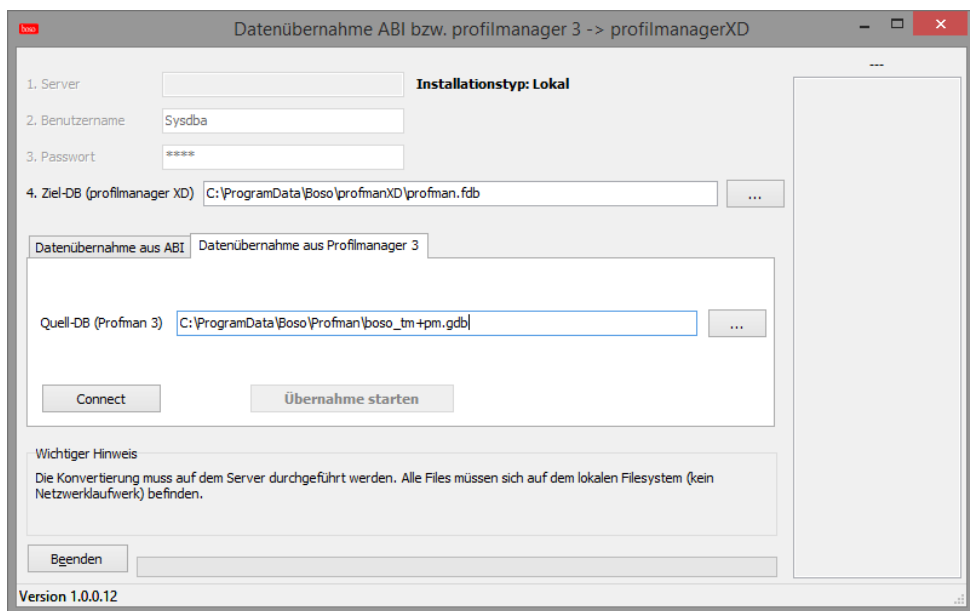


If you transfer data from both ABI and profil-manager 3, the separate sets of data are brought together in the new database.

Measurements for a specific patient are only brought together if the surname, first name and date of birth are the same. If the patient numbers are different, the patient number of the target database is retained.

If the surname, first name and date of birth do not match, or if these fields are empty or out of date, a new patient record will be created. The patient number is retained unless it already exists in the target database, in which case a new patient number will be created.

All patients with mismatches are transferred to a list. The data can be updated before being transferred. Missing or out-of-date data will not be transferred (screenshot in German).

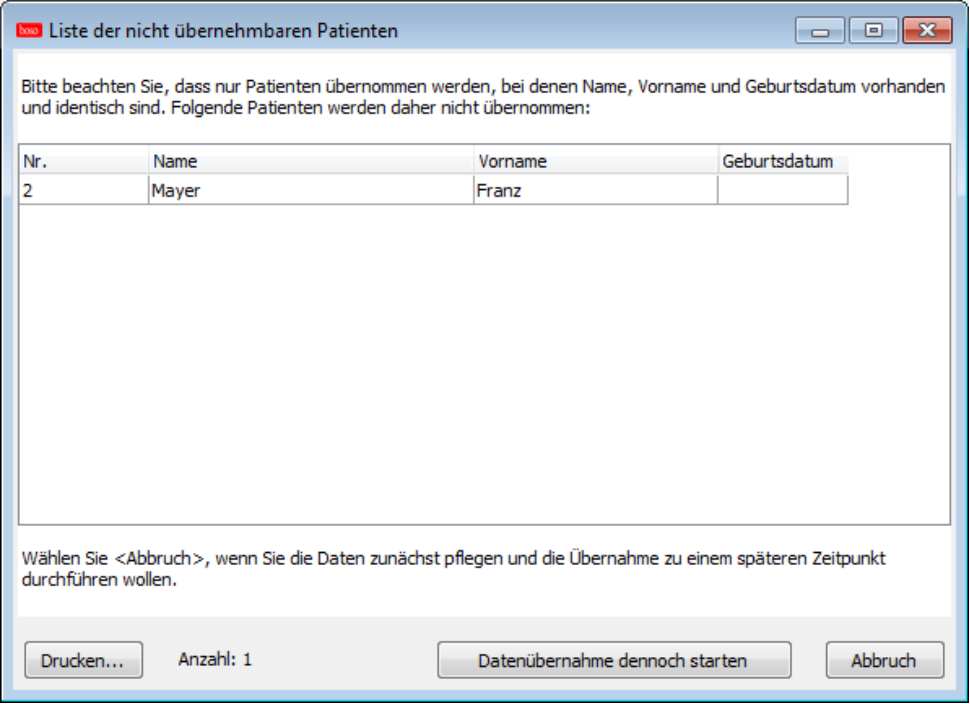


1.4 Installing the USB connection cable


If the USB driver was pre-installed during installation (this is normally the case), you simply need to plug the USB connection cable provided into a free USB port. The cable is then automatically recognised and installed.

If the driver was not pre-installed, you must execute the file dpinst_32bit.exe (present after installation in the directory C:\Programme\Boso\profmanXD\ftdi\) as administrator and then plug the USB cable into a free USB port.


2. Start

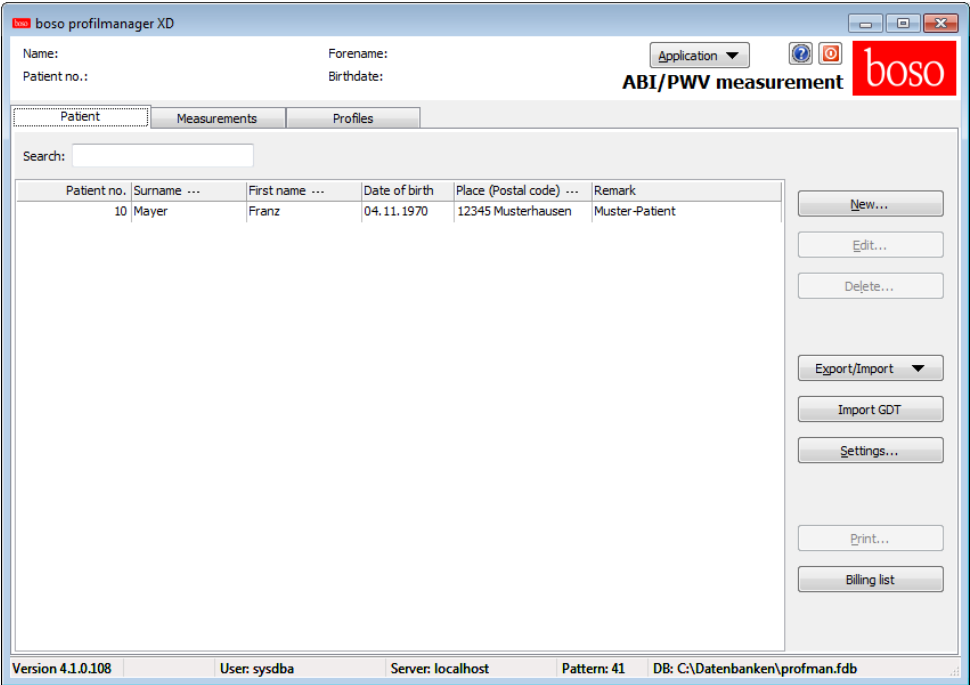

After starting boso profil-manager XD by clicking on the "boso profil-manager XD" icon, select the part of the program you wish to run in the light of the device application you are currently using:

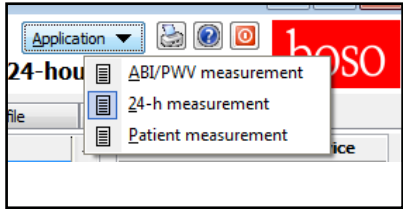


Applications with data already stored are indicated by the  symbol.

Applications with no data at present are indicated by the  symbol.

If you switch from one application to another for a selected patient, the "Measurements" registry is automatically selected. This means that measurements from various applications provide you with an overall view of all measurements for a particular patient.

Accessing the help function

Press the F1 key or  button to call up these and other instructions for use in PDF format at any time.

2.1 Patient registry, for all applications

Click on a patient to select him or her.

Patients can be sorted by clicking on the header of the relevant column.

Use the “Restore column order” function to go back to the original sorting by patient number. To do this, right-click in the header row of the patient table.

You can search by name via the “Search” function.

2.1.1 “New...” button

This sets up a new patient. The name and patient number fields must be completed. The system will suggest a patient number, but you can change this manually.

2.1.1 “Modify...” button

This alters an existing patient’s personal data.

2.1.1 “Delete...” button

This deletes a patient.



This process is irreversible: all data (including measurements from all parts of the application) are deleted and cannot be recovered.

2.1.4 “Export/Import” button

2.1.4.1 “Export Excel” exports data for the currently selected patient (from the current ABI, 24-hour, patient measurement application) in Excel-readable .xls format. You can choose whatever file name and storage location you like.

2.1.4.2 “Export patient (XML)” exports data for the currently selected patient in profil-manager XD-readable .xml format.

2.1.4.3 "Import Patient (XML)" imports data for a selected patient.

The following rules apply to 2.1.4.2 and 2.1.4.3:

The transfer path from the transfer file settings is used for incorporation into the clinic's data processing system (see next chapter, "Settings..." button)

The file name is made up of the active application and the patient number.
For example, "2430_10.xml" stands for patient data for the patient with patient number 10 from the 24-hour measurement application.

2430_#.xml stands for data from the 24-hour measurement
ABI_#.xml stands for data from the ABI measurement
medicus_#.xml stands for data from patient measurement

2.1.5 Import GDT

The GDT-import file, if available, is read and the included patient is selected or created. If a patient with the imported patient number already exists, the following screen appears.

Do you want to select this patient?

Personal Data

Name

Mayer

Forename

Franz

Date of birth

04.11.1970

dd.mm.yyyy

☒ Male

☐ Female

Other

Patient No.

10

Insurance No.

Address

Street

Musterstraße 99

Zip / City

12345 Musterhausen

Dimensions

Height

175,5

cm

Weight

75,5

kg

Remarks


Muster-Patient

Yes, select this patient

No, use patient data from GDT import

Cancel

The button "Yes, select this patient" selects the indicated patient.



With the button "No, use patient data from GDT import" all existing data will be assigned to the patient from the GDT import file.

2.1.6 “Settings” button

The settings are explained in the sections dealing with particular applications (chapters 3 to 5) as they are application-specific.

2.1.7 “Print...” button

Patient data is presented on screen (preview), printed out on the printer selected under “Setup”, and/or in the configured PDF file.

The Windows standard printer is the default for print-outs.

If you selected “PDF file” in the printer settings, a PDF file will be created. The name of this PDF file is pmXD_pat#.pdf

Where

pat#=patient number

2.1.8 “Billing assistance...” button

This creates a summary of the number of measurements in the currently selected application that have been performed within a given time period (not available for patient measurement).

For example, this provides a simple indication of how many 24-hour measurements were performed in the first quarter.

If you selected “PDF file” in the printer settings, a PDF file will be created. The name of this PDF file is pmXD_cl.pdf.


3. "ABI/PWV measurement" application

3.1 "Patient" registry

see section "2.1 Patient registry, for all applications"

See chapter 3.4 for "Settings" button

3.2 "Measurements" registry

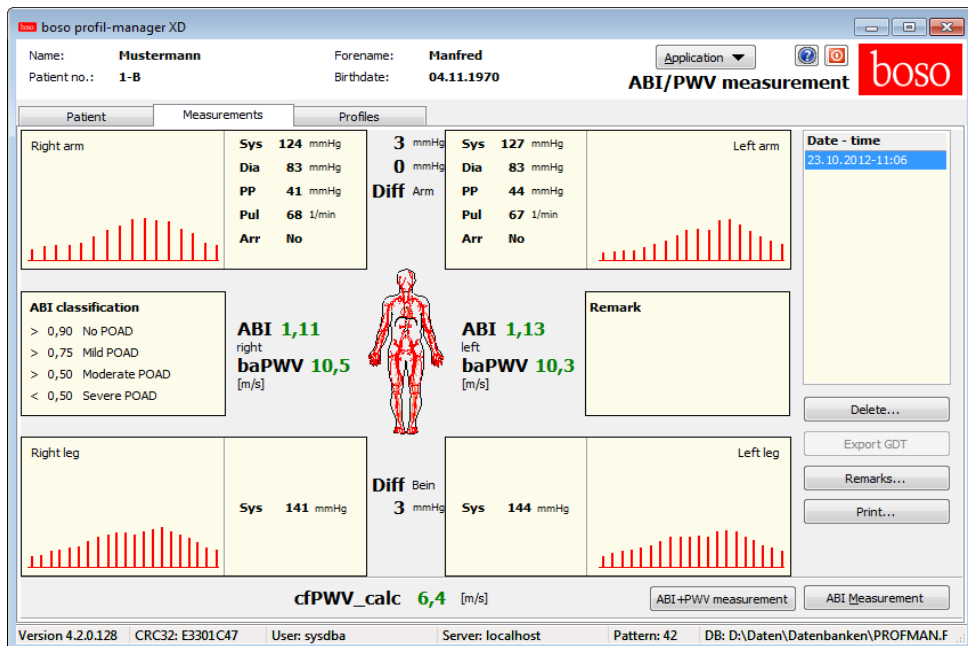

Measurements that have been carried out can be viewed, and new measurements can be performed, in the "Measurements" registry.

To display ABI / PWV measurements that have already been carried out, select the desired ABI / PWV measurements in the "Date-Time" field.

The screen displays the following parameters (for the left and right half of the body in each case):

Sys upper arm systolic blood pressure, with measurements >140 mmHg in red

Dia upper arm diastolic blood pressure, with measurements >90 mmHg in red

PP pulse pressure = difference between systole and diastole, with measurements >54 mmHg in red

Pul pulse in 1/min

Arr Indication of whether a pulse irregularity of over 25% was observed during the measurement. Display in red indicates arrhythmia.

ABI Ankle-brachial index = ratio of the systolic pressure measured in the leg and the higher systolic pressure measured in the arm. Display in red indicates an ABI < 0.9 [default].

baPWV (optional) measured pulse wave velocity brachial-ankle, displayed in red indicates $\geq 14,5$ m/s.

cfPWV_calc (optional) pulse wave velocity carotid-femoral calculated from baPWV, displayed in red indicates ≥ 10 m/s. (No calculation if both ABI < 0.9)



The patient's height must be recorded as this information is needed to calculate PWV.

Sys systolic blood pressure in the ankle



Note the information on page 25.

Diff Arm Sys Difference between the systolic values in the left and right upper arms, with results > 10mmHg displayed in red

Diff Arm Dia Difference between the diastolic values in the left and right upper arms, with results > 10mmHg displayed in red

Diff Leg Sys Difference between the systolic values in the left and right ankles, with results > 10mmHg displayed in red.

Clicking on one of the oscillation profiles enlarges the selected profile. The “pulse level over time” registry shows the course of oscillation over the time axis. The “pulse level over cuff pressure” registry shows the course of oscillation over cuff pressure.

3.2.1 “Delete” button


Measurements that have already been performed can be irrevocably deleted by this button.

3.2.2 “Export GDT” button

This generates the GDT export file manually. Only available if the GDT import of the active patient has already been performed.


3.2.3 “Remarks...” button

Click in the “Remarks” field or the “Remarks” button to add a remark to a measurement.

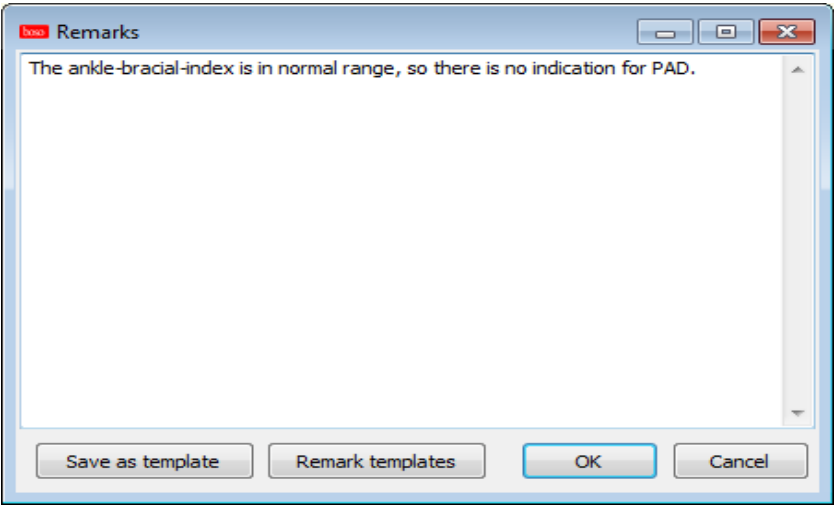

Remarks that are made frequently can be stored as templates using the “Store as template” button. You can use the “Remark templates” button to easily insert stored remark templates into a remark field at any time.

Measurements with remarks are marked with an “R” in the “Date-Time” field.



3.2.47 “Print” button

This produces a print-out of the current measurement.

If you selected “PDF file” in the printer settings, a PDF file will be created. The name of this PDF file is ABI_pat#_YYYYMMDD_m.pdf

where

pat#=patient number
YYYYMMDD = date of measurement
m = measurement reference letter

3.2.5 “ABI measurement” button

This initialises the boso ABI system 100 and starts a new measurement.

You can cancel a measurement which is being performed at any time by using the “Cancel measurement” button or pressing the STOP key on the device.

Once the measurement of a limb has been completed, the “Store measurement” key is activated.

You could store the measurement at this stage (for example, if the patient has a limb missing).

Once all measurements on four limbs have been completed, a green border appears around the active “Store measurement” button. This indicates that the measurements have been successfully completed and can be stored.

If an error occurs during a measurement, the following error message appears in the corresponding measurement window:

(82) measurement error -> retry measurement.



If this error occurs repeatedly, this can indicate that the patient has a vascular disease. Further investigation is recommended in this case once a technical defect has been ruled out. If no reading is displayed for systolic blood pressure **in the ankle**, check the cuff and tubes and then retry. If no reading is displayed the second time, this can indicate a circulation disorder or medial sclerosis. Here again further investigations are recommended.

(83) Connect cuff

(89) System error -> Device should be checked by the manufacturer’s technical support service

3.2.6 “ABI+PWV measurement” button (optional)

This automatically performs a PWV measurement 10 seconds after completion of the ABI measurement described under 3.2.5.


A green border appears around the “Store measurement” button once the PWV measurement has been completed. This indicates that the PWV measurement has been successfully completed and can be stored.

3.3 “Profiles” registry



The ABI values (and PWV values if this option is selected) of all measurements are presented in the form of bar charts in the “Profiles” registry. The ABI colour display is as per the setting under “Classification” (red: ABI < 0.9).

Various parameters are available to alter the optical presentation of the profile:

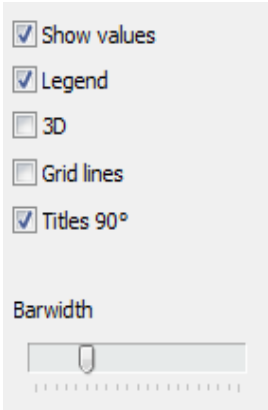

Display values (standard): ABI values are displayed above the bars.

Legend: The legend for the readings is displayed in the diagram.

3D: The bars are displayed in 3D.

Grid lines: Grid lines are shown in the coordinates system.

90° title: The title of the x-axis is rotated through 90°.

3.3.1 “Print” button

This produces a print-out of the profile display.

If you selected “PDF file” in the printer settings, a PDF file will be created. The name of this PDF file is ABI_pat#_p.pdf


where

pat#=patient number

p = profile reference letter

3.4 “Settings...” button in “Patient” registry

3.4.1 “Doctor” sub-registry

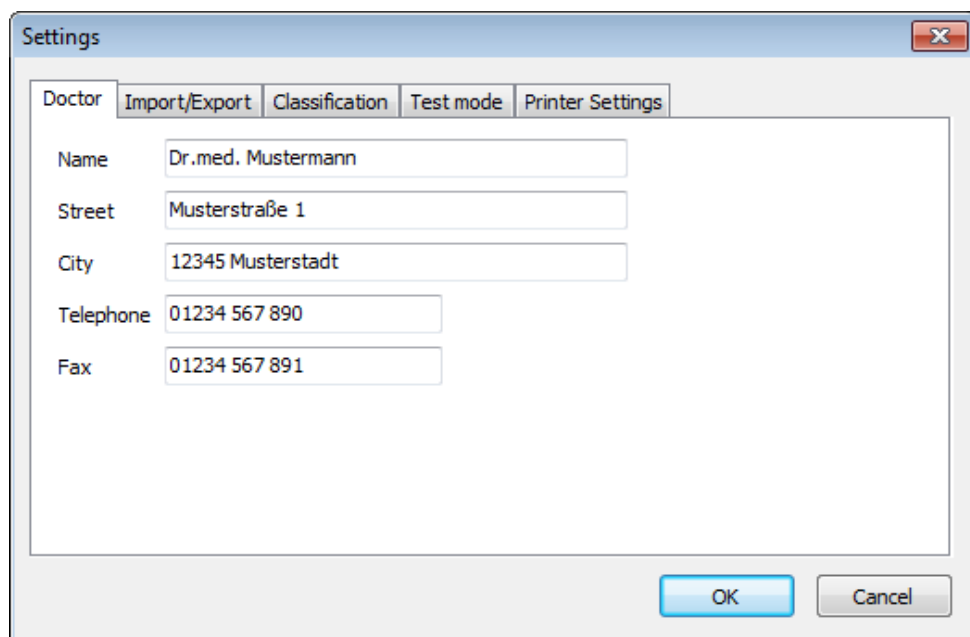


The screenshot shows a 'Settings' dialog box with a tabbed interface. The 'Doctor' tab is selected, showing input fields for Name, Street, City, Telephone, and Fax. The other tabs are 'Import/Export', 'Classification', 'Test mode', and 'Printer Settings'. The 'OK' and 'Cancel' buttons are at the bottom right.

Field	Value
Name	Dr.med. Mustermann
Street	Musterstraße 1
City	12345 Musterstadt
Telephone	01234 567 890
Fax	01234 567 891

The personal details of the doctor treating the patient are entered in the “Doctor” registry and used to produce the footer in the print-out.

3.4.2 "Import/Export" sub-registry

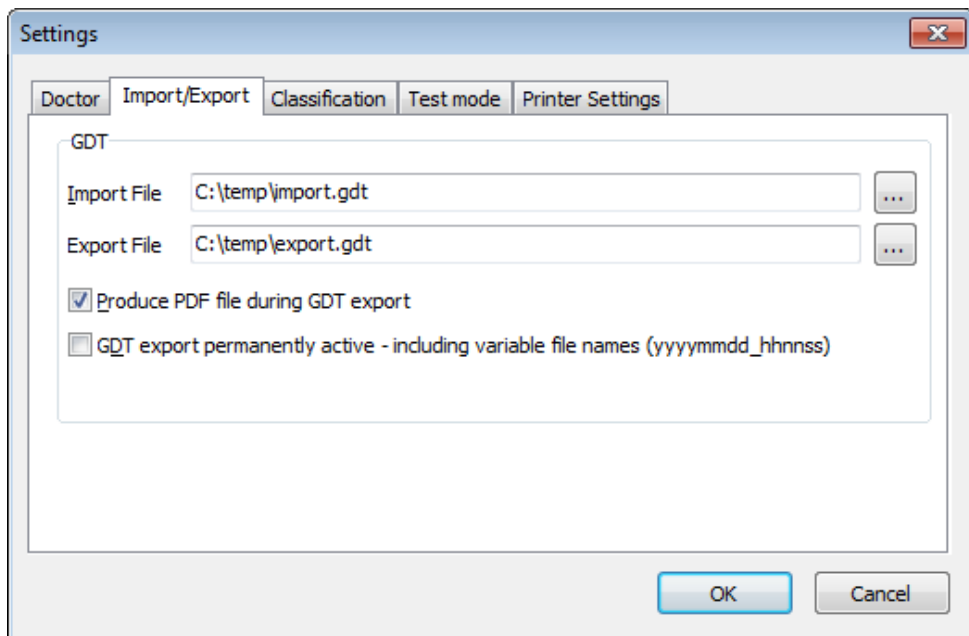

The screenshot shows a 'Settings' window with a tabbed interface. The 'Import/Export' tab is selected. Inside this tab, there is a section titled 'GDT'. It contains two text input fields: 'Import File' with the value 'C:\temp\import.gdt' and 'Export File' with the value 'C:\temp\export.gdt'. Each field has a button with three dots to its right for file selection. Below these fields are two checkboxes: the first is 'Produce PDF file during GDT export' which is checked, and the second is 'GDT export permanently active - including variable file names (yyyyMMdd_hhnnss)' which is unchecked. At the bottom right of the window are 'OK' and 'Cancel' buttons.

If you are using a clinic data processing system that supports the GDT interface, this is where the path and file names for export and import files are set. You have direct access to the Windows directory structure via the buttons next to the input fields for import and export files.

For example: c:\prax_ed\import.gdt
Import file = clinic DP system export file
Export file = clinic DP system import file

GDT import takes place automatically when you start the program, or manually by clicking the "Export/Import -> Import GDT" button if a valid GDT import file is present in the relevant directory.

GDT export takes place only if the patient being imported from the clinic DP system is active. Export takes place automatically when the program is closed down (if measurements have been read in from the device during the current program session) or can be performed manually at any time by clicking the "Export GDT" button in the "Measurements" registry.



Data export is deactivated if another patient has been selected after automatic import. It is reactivated when the first patient is reselected. Data export is also deactivated if no import has first taken place.

For certain applications (e.g. HL7 in hospital), it may be necessary to activate GDT-export permanently and name the export file variable (Export.gdt -> yyyyymmdd_hhmmss.gdt). For this, activate the option "GDT export is permanently active - including variable file name".



If this option is selected, precautions must be taken (check patient number) to avoid incorrect allocation of readings.

With the active option "produce PDF file during GDT export" a PDF-file is created with the GDT export.

3.4.3 "Classification" sub-registry


Symbol	Value	Classification
>	0,90	No PAOD
>	0,75	Mild PAOD
>	0,50	Moderate POAD
<	0,50	Severe PAOD

Limits for ABI value classification can be amended here.



Modifications do not take effect until the program is restarted.

3.4.4 “Test mode” sub-registry

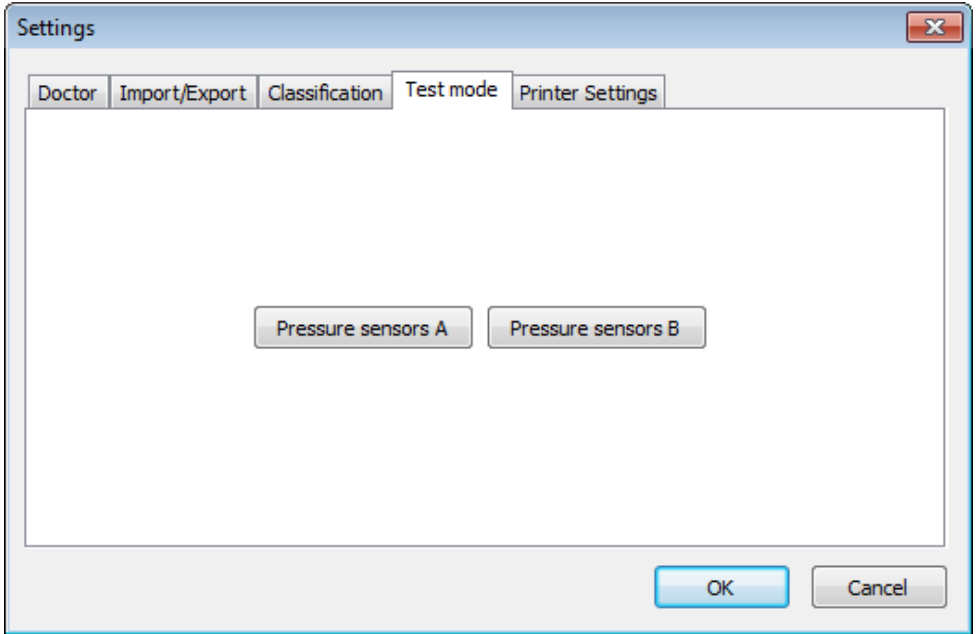

Clicking on the “pressure sensors A” or “pressure sensors B” button switches the ABI system 100 into test mode. Clicking on the “End test” button ends test mode. This function is needed for various purposes, for example testing pressure during metrology tests.


(optional)

Special simulators are needed to perform functional tests of the device with the “PWV” option, and these tests must be carried out on the manufacturer's premises.



The activation of the “pressure sensors B” is only possible for devices with a serial number upper 466 20000.

3.4.5 “Printer settings” sub-registry

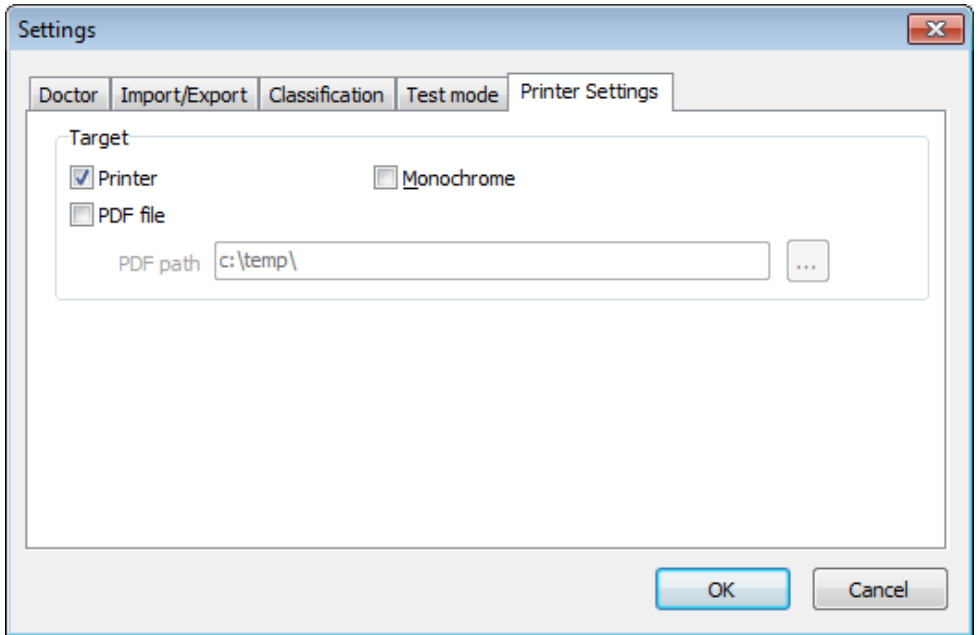

In the “Printer settings” registry you decide whether the print-out should be produced in paper form, as a screen print and/or as a PDF document, once the relevant [Print...] buttons have been clicked while the program is running.

If you select “Printer”, then the “Output Options” dialogue appears when you click on the [Print...] buttons while the program is running. You can choose either a print output (“Printer”) or a screen view (“Preview”).

If you select “PDF file”, a PDF file is produced. The name of this PDF file is created in different ways depending on the application, and this process is described in more detail in the individual applications.



You must select at least one medium: “Printer” or “PDF file”.

If you select the “monochrome” option, the print will be in black and white.

4. "24-hour measurement" application

4.1 "Patient" registry

see section "2.1 Patient registry, for all applications"

See chapter 4.7 for "Settings" button.


4.2 "Measurements" registry

The screenshot displays the 'boso profilmanager XD' application window. At the top, patient information is shown: Name: Mayer, Forename: Franz, Patient no.: 10, Birthdate: 04.11.1970. The 'Application' dropdown is set to 'Patient measurement'. The main data table is titled 'Measurements' and contains 22 rows of data, each representing a measurement taken at a specific time and date. The columns are: Date, SYS, DIA, PUL, MAP, PP, Arr., Exclude, and Remark. The 'Exclude' column has checkboxes, with the last row (22 So, 17.04.2005 - 08:22) checked. To the right of the table is a 'Period' and 'Device' section, showing the selected period as '06.04.2005 - 27.06.2005' and the device as 'medlife PC3'. Below this are buttons for 'Delete Period...', 'Export GDT', 'Manual Data...', 'Print...', 'Transfer Data...', and 'Interval limits...'. At the bottom, there are filters for 'All', 'Morning', and 'Afternoon', and a date range selector set to '01.01.2012' to '31.12.2012'. The status bar at the very bottom shows 'Version 4.1.0.108', 'User: sysdba', 'Server: localhost', 'Pattern: 41', and 'DB: C:\Datenbanken\profman.fdb'.

	Date	SYS	DIA	PUL	MAP	PP	Arr.	Exclude	Remark
1	Mi, 06.04.2005 - 18:26	144	75	65	98	69		<input type="checkbox"/>	Test
2	Do, 07.04.2005 - 08:32	159	88	68	112	71		<input type="checkbox"/>	
3	Do, 07.04.2005 - 18:37	153	92	67	112	61		<input type="checkbox"/>	
4	Fr, 08.04.2005 - 08:44	164	76	72	105	88		<input type="checkbox"/>	
5	Fr, 08.04.2005 - 18:49	152	87	68	109	65		<input type="checkbox"/>	
6	Sa, 09.04.2005 - 08:54	176	87	67	117	89		<input type="checkbox"/>	
7	Sa, 09.04.2005 - 18:59	160	99	67	119	61		<input type="checkbox"/>	
8	So, 10.04.2005 - 08:04	146	80	68	102	66		<input type="checkbox"/>	
9	So, 10.04.2005 - 18:09	153	82	66	106	71		<input type="checkbox"/>	
10	Mo, 11.04.2005 - 08:16	156	91	61	113	65		<input type="checkbox"/>	
11	Mo, 11.04.2005 - 18:20	160	84	65	109	76		<input type="checkbox"/>	
12	Di, 12.04.2005 - 08:28	151	88	60	109	63		<input type="checkbox"/>	
13	Di, 12.04.2005 - 18:34	152	81	64	105	71		<input type="checkbox"/>	
14	Mi, 13.04.2005 - 08:39	152	81	65	105	71		<input type="checkbox"/>	
15	Mi, 13.04.2005 - 18:46	177	86	62	116	91		<input type="checkbox"/>	
16	Do, 14.04.2005 - 08:51	161	89	60	113	72		<input type="checkbox"/>	
17	Do, 14.04.2005 - 18:57	163	86	70	112	77		<input type="checkbox"/>	
18	Fr, 15.04.2005 - 08:02	174	92	67	119	82		<input type="checkbox"/>	
19	Fr, 15.04.2005 - 18:07	166	96	71	119	70		<input type="checkbox"/>	
20	Sa, 16.04.2005 - 08:12	164	91	64	115	73		<input type="checkbox"/>	
21	Sa, 16.04.2005 - 18:17	148	91	70	110	57		<input type="checkbox"/>	
22	So, 17.04.2005 - 08:22	138	91	70	107	47		<input checked="" type="checkbox"/>	

All measurements that have been read in to date for the selected patient are displayed here.

This is where the TM-2430 is initialised and data is read out from the device.
A patient must be selected before you can switch to this registry. When the program starts, no patient is selected. If you have not selected a patient manually, or imported a patient automatically via the GDT interface, you will see this help mask:

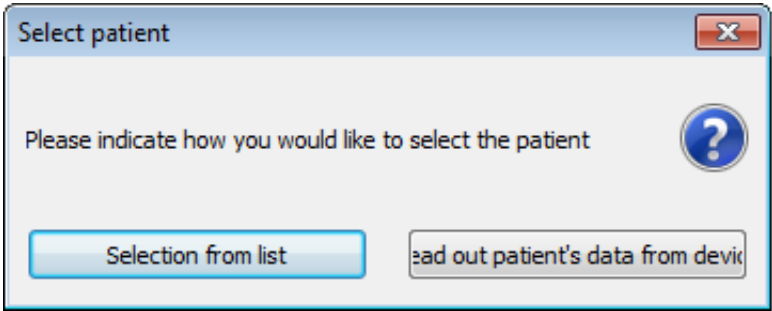

The "Select from list" button shows you a list of all available patients so that you can select the appropriate patient manually.

The "Read out patient from device" button identifies the patient you want to select via the patient number stored in the device.

Both the period and the blood pressure meter with which the series of measurements was carried out are displayed.

Select the appropriate period.

Period	Device
12.01.2006 - 13.01.2006	TM-2430
02.11.2005 - 03.11.2005	TM-2430

	Date	SYS	DIA	PUL	MAP	PP	Arr.	Exclude	Remark
1	Mi, 06.04.2005 - 18:26	144	75	65	98	69		<input type="checkbox"/>	Test
2	Do, 07.04.2005 - 08:32	159	88	68	112	71		<input type="checkbox"/>	
3	Do, 07.04.2005 - 18:37	153	92	67	112	61		<input type="checkbox"/>	
4	Fr, 08.04.2005 - 08:44	164	76	72	105	88		<input type="checkbox"/>	
5	Fr, 08.04.2005 - 18:49	152	87	68	109	65		<input type="checkbox"/>	
6	Sa, 09.04.2005 - 08:54	176	87	67	117	89		<input type="checkbox"/>	
7	Sa, 09.04.2005 - 18:59	160	99	67	119	61		<input type="checkbox"/>	
8	So, 10.04.2005 - 08:04	146	80	68	102	66		<input type="checkbox"/>	
9	So, 10.04.2005 - 18:09	153	82	66	106	71		<input type="checkbox"/>	
10	Mo, 11.04.2005 - 08:16	156	91	61	113	65		<input type="checkbox"/>	
11	Mo, 11.04.2005 - 18:20	160	84	65	109	76		<input type="checkbox"/>	
12	Di, 12.04.2005 - 08:28	151	88	60	109	63		<input type="checkbox"/>	
13	Di, 12.04.2005 - 18:34	152	81	64	105	71		<input type="checkbox"/>	
14	Mi, 13.04.2005 - 08:39	152	81	65	105	71		<input type="checkbox"/>	
15	Mi, 13.04.2005 - 18:46	177	86	62	116	91		<input type="checkbox"/>	
16	Do, 14.04.2005 - 08:51	161	89	60	113	72		<input type="checkbox"/>	
17	Do, 14.04.2005 - 18:57	163	86	70	112	77		<input type="checkbox"/>	
18	Fr, 15.04.2005 - 08:02	174	92	67	119	82		<input type="checkbox"/>	
19	Fr, 15.04.2005 - 18:07	166	96	71	119	70		<input type="checkbox"/>	
20	Sa, 16.04.2005 - 08:12	164	91	64	115	73		<input type="checkbox"/>	
21	Sa, 16.04.2005 - 18:17	148	91	70	110	57		<input type="checkbox"/>	
22	So, 17.04.2005 - 08:22	138	91	70	107	47		<input checked="" type="checkbox"/>	
1	2	3	4	5	6	7	8	9	10

The column content is as follows:

- 1: serial numbers of measurements
- 2: date and time of measurement
- 3: SYS = systolic blood pressure
- 4: DIA = diastolic blood pressure
- 5: PUL = pulse
- 6: MAP = mean arterial blood pressure, calculated as $DIA + 1/3 \text{ pulse pressure}$
- 7: PP = pulse pressure (SYS – DIA)
- 8: Exclude = if you highlight this, the measurement will not be taken into account for assessment in the profile and statistics
- 9: S = measurement performed at night
- 10: Remark. Double-click in the measurement line to add a remark to a measurement. This opens the remark input field:

Process remark

Date: 06.04.2005 Time: 18:26

Sys: 144
Dia: 75
Puls: 65
MAP: 98
PP: 69

Remark: Test

OK Cancel

4.2.1 “Delete period” button

This irrevocably deletes a complete set of readings.

4.2.2 “Export GDT” button

This generates the GDT export file manually. Only available if the GDT import of the active patient has already been performed.

4.2.3 “Manual data” button

This allows you to add new readings to the active set of readings, or process or delete them.

4.2.4 “Print...” button

This prints out the list of readings.
If you selected “PDF file” in the printer settings (chapter 4.7.3), a PDF file will be created.
The name of this PDF file is `tm_pat#_YYYYMMDD_m.pdf`

where
 pat#=patient number
 YYYYMMDD = date of measurement
 m = measurement reference letter

4.2.5 “Initialise” button

TM-2430 Settings

Patient **Mayer, Franz**

Mode

- ☒ Standard Settings (Periods/Intervals)
- ☐ Sleep Button
- ☐ User Settings (Periods/Intervals)

Date/Time

Current System Time 11.07.2012 15:41

TM-2430 Time 11.07.2012 15:40

Periods/Intervals

	Day	Night
Start of Period	7 :00	22 :00
Interval	15	30

Actions

Apply System Time ☒

Display on ☒

Miscellaneous

Max. inflation Press. 300 mmHg

OK Cancel

The TM-2430 device can be initialised with a unique patient number up to 10 characters in length. The benefit of this is that measurements can be immediately assigned to the correct patient when they are read out.

The current patient is automatically transferred to the programming window, and the patient number is assigned to the device (the software generates a numerical identifier, which means that alphanumeric patient numbers can also be used in profil-manager XD).

You can specify a maximum inflation pressure in the “Max. infl. press.” field. The blood pressure meter will then not inflate beyond the figure you have set here.



If the patient’s systolic blood pressure is close to or above this figure, it will not be possible to measure blood pressure. The device then produces an error message.




The patient number programming and pressure restriction features are not available on TM-2430 devices with serial numbers below SN M 0713550.

Three different modes can be programmed.

Standard periods / intervals

When this mode is selected, the device takes a reading every 15 minutes between 7 a.m. and 10 p.m., and every 30 minutes between 10 p.m. and 7 a.m.

Sleep button

In this mode the patient can decide when the night and day intervals should begin, by pressing the black button  on the TM-2430 blood pressure meter. The benefit of this programming feature is that it allows measurement intervals to be tailored to the patient. For example, for patients with irregular sleep patterns.

The interval durations are 15 minutes (day interval) and 30 minutes (night interval).

Programmable periods / intervals

Two intervals and periods can be programmed according to individual preference in this mode. The interval duration can be set as 5, 10, 20, 30, 60 or 120 minutes.

Display reading

Activating or deactivating this command determines whether or not the reading is displayed after the measurement has been performed.


Set system time

Activating this command transfers the date and time settings on your PC.


4.2.6 "Transfer data" button

Connect the meter to the PC connection cable before activating the "data transfer" button. Measurements are transferred from the meter which is connected. Once data has been transferred, the interval limits can be adapted individually to the patient's actual daily routine by clicking the "Modify" button.

Clicking the "Yes" button clears the device's data memory.

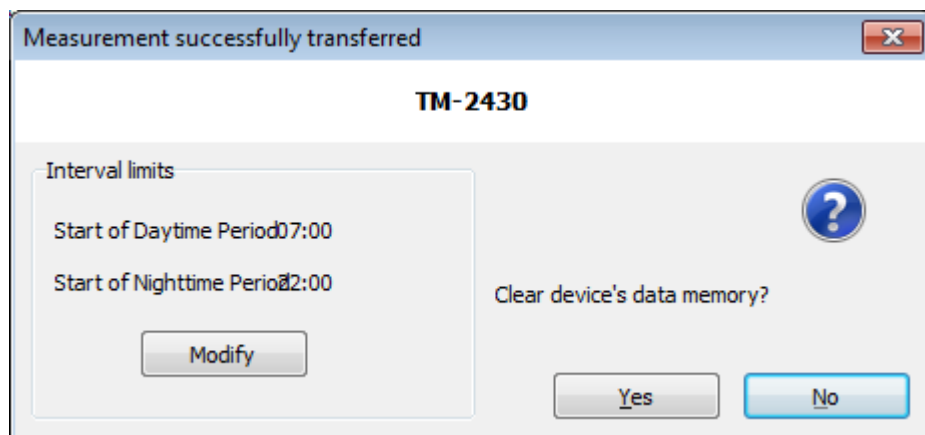

4.3 “Sys/dia profile” registry

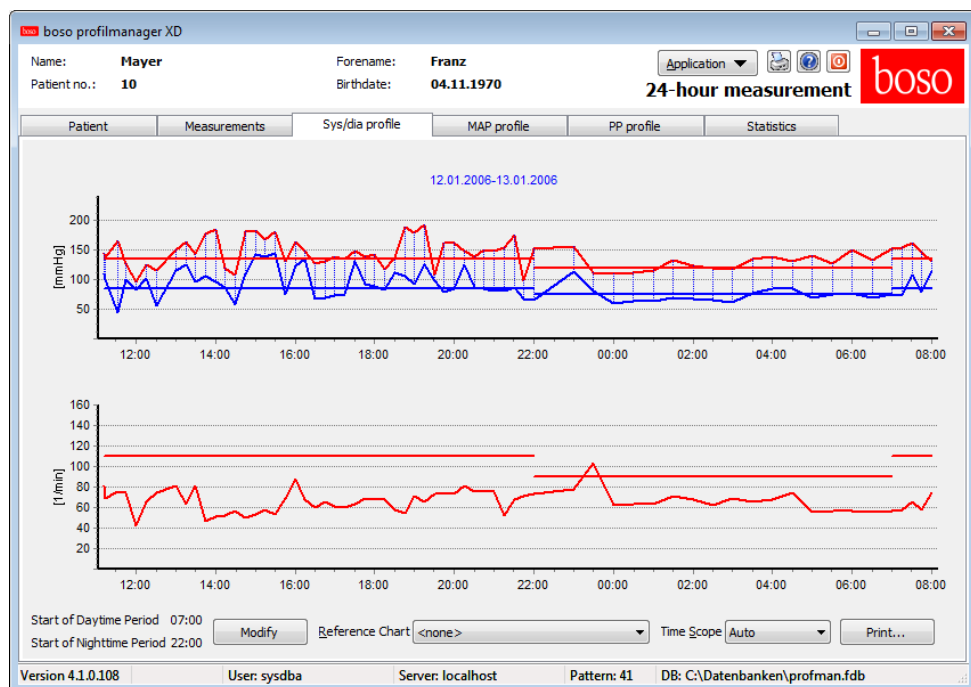

This displays the blood pressure trend.

The pulse trend can be displayed or hidden by the Ctrl+P key combination.

Move the cursor over the measurement to obtain more information about individual readings. The date, time and reading are displayed in the top left-hand corner of the diagram.

4.3.1 “Modify” button

Interval limits can be adapted individually to the patient's actual daily routine by clicking the “Modify” button.

4.3.2 “Reference Chart” button

Clicking this reads in data from an additional 24-hour measurement into the current graph, so that the two sets of measurements can be compared directly.

4.3.3 "Time scope" selection field

This allows you to select the period for which measurements are displayed. You have the choice of Auto or Day.

"Auto" is the default setting. In this setting, the time scope is scaled from the first measurement to the last.

In the "Day" setting, exactly 24 hours are displayed.

Right-clicking in the diagram allows you to shift the graph horizontally with the mouse.

4.3.4 "Print..." button

This produces a print-out of the SYS/DIA profile, pulse profile and statistics.

If you selected "PDF file" in the printer settings (chapter 4.7.3), a PDF file will be created. The name of this PDF file is tm_pat#_YYYYMMDD_sys.pdf


where

pat#=patient number

YYYYMMDD = date of measurement

SYS/DIA reference letter

4.4 “MAP profile” registry

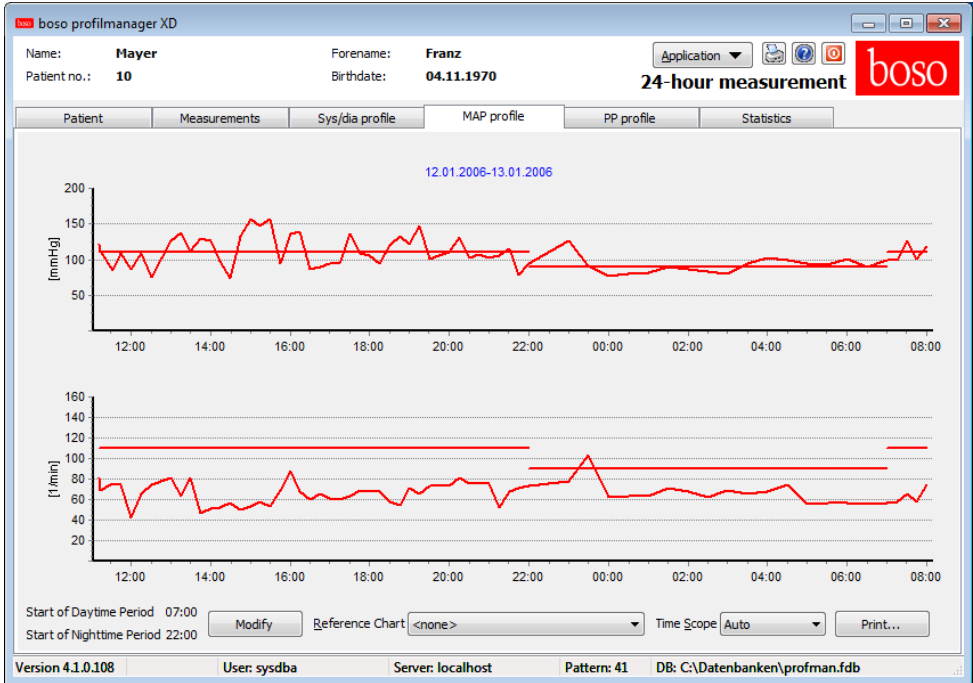

This displays the trend for the calculated mean arterial blood pressure.
(MAP = diastole DIA + 1/3 pulse pressure PP)

The pulse trend can be hidden or displayed by the Ctrl+P key combination.

Move the cursor over the measurement to obtain more information about individual readings. The date, time and reading are displayed in the top left-hand corner of the diagram.

4.4.1 “Modify” button

Interval limits can be adapted individually to the patient's actual daily routine by clicking the “Modify” button.

4.4.2 “Reference Chart” selection field

Clicking this reads in data from an additional 24-hour measurement into the current graph, so that the two sets of measurements can be compared directly.

4.4.3 "Time scope" selection field

This allows you to select the period for which measurements are displayed. You have the choice of Auto or Day.

"Auto" is the default setting. In this setting, the time scope is scaled from the first measurement to the last.

In the "Day" setting, exactly 24 hours are displayed.

Right-clicking in the diagram allows you to shift the graph horizontally with the mouse.

4.4.4 "Print..." button

This produces a print-out of the MAP profile, pulse profile and statistics.

If you selected "PDF file" in the printer settings (chapter 4.7.3), a PDF file will be created. The name of this PDF file is tm_pat#_YYYYMMDD_map.pdf


where

pat#=patient number

YYYYMMDD = date of measurement

map = MAP reference letter

4.5 “PP profile” registry

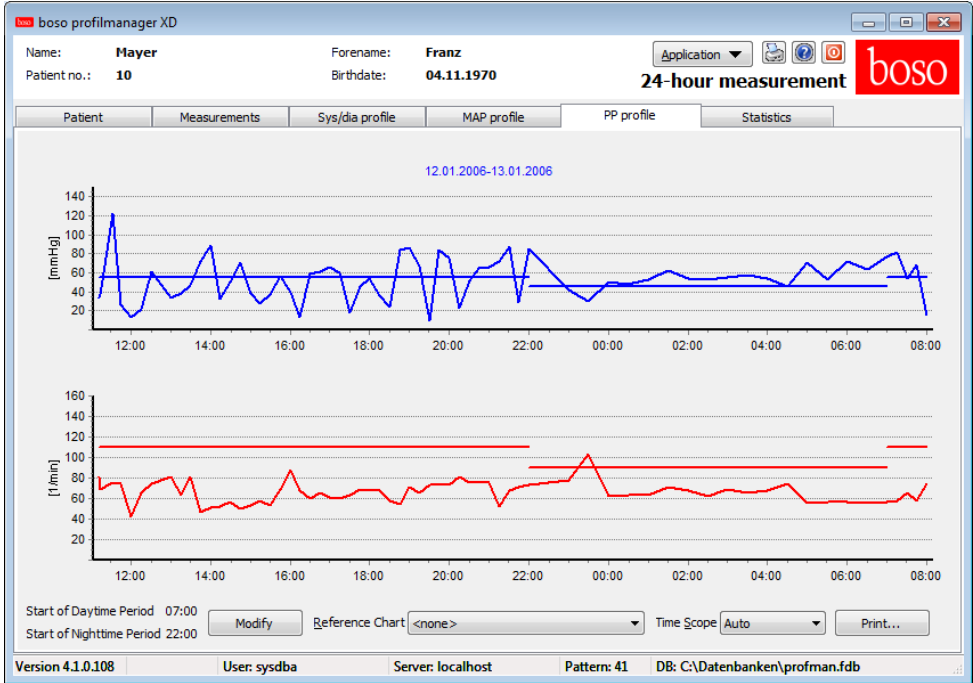

This displays the trend for the calculated pulse pressure. (PP = SYS-DIA)

The pulse trend can be hidden or displayed by the Ctrl+P key combination.

Move the cursor over the measurement to obtain more information about individual readings. The date, time and reading are displayed in the top left-hand corner of the diagram.

4.5.1 “Modify” button

Interval limits can be adapted individually to the patient's actual daily routine by clicking the “Modify” button.

4.5.2 “Reference Chart” selection field

Clicking this reads in data from an additional 24-hour measurement into the current graph, so that the two sets of measurements can be compared directly.

4.5.3 “Time scope” selection field

This allows you to select the period for which measurements are displayed. You have the choice of Auto or Day.

“Auto” is the default setting. In this setting, the time scope is scaled from the first measurement to the last.

In the “Day” setting, exactly 24 hours are displayed.

Right-clicking in the diagram allows you to shift the graph horizontally with the mouse.

4.5.4 “Print...” button

This produces a print-out of the pulse pressure profile, pulse profile and statistics. If you selected “PDF file” in the printer settings (chapter 4.7.3), a PDF file will be created.

The name of this PDF file is tm_pat#_YYYYMMDD_pp.pdf


where

pat#=patient number

YYYYMMDD = date of measurement

pp = pulse pressure reference letter

4.6 “Statistics” registry

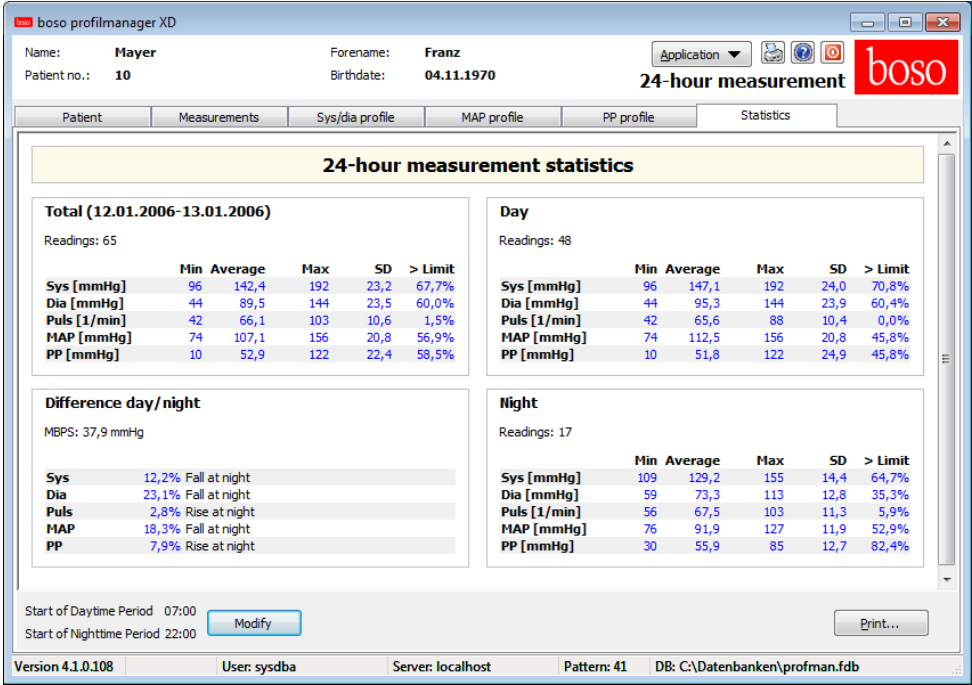

Measurements for the total period, daytime and nighttime periods are assessed separately.

The total value of the readings is displayed in the individual periods.

The following values are shown in the individual columns:

Min: smallest value in the interval in question

Mean: arithmetic mean in the interval in question

Max: largest value in the interval in question

SD: standard deviation in the interval in question

> Limit: percentage above the limits that have been set

MBPS: morning blood pressure surge

The MBPS indicates the rise in blood pressure after getting up.

$MBPS = MwSysDay - MwSysNight$

where

$MwSysDay$ = average of systolic values in the first two hours of the daytime interval

MwSysNight = average of the three systolic values surrounding the lowest systolic value in the nighttime interval (one value before the lowest value, the lowest value itself and one value after the lowest value).

The percentage increase/decrease during the night is displayed.

4.6.1 "Modify" button

Interval limits can be adapted individually to the patient's actual daily routine by clicking the "Modify" button.

4.6.2 "Print..." button

This produces a print-out of the SYS/DIA profile, pulse profile and statistics.

If you selected "PDF file" in the printer settings (chapter 4.7.3), a PDF file will be created. The name of this PDF file is tm_pat#_YYYYMMDD_sys.pdf

where


pat#=patient number

YYYYMMDD = date of measurement

sys = SYS/DIA reference letter

4.7 “Settings...” button in “Patient” registry

4.7.1 “Doctor” sub-registry

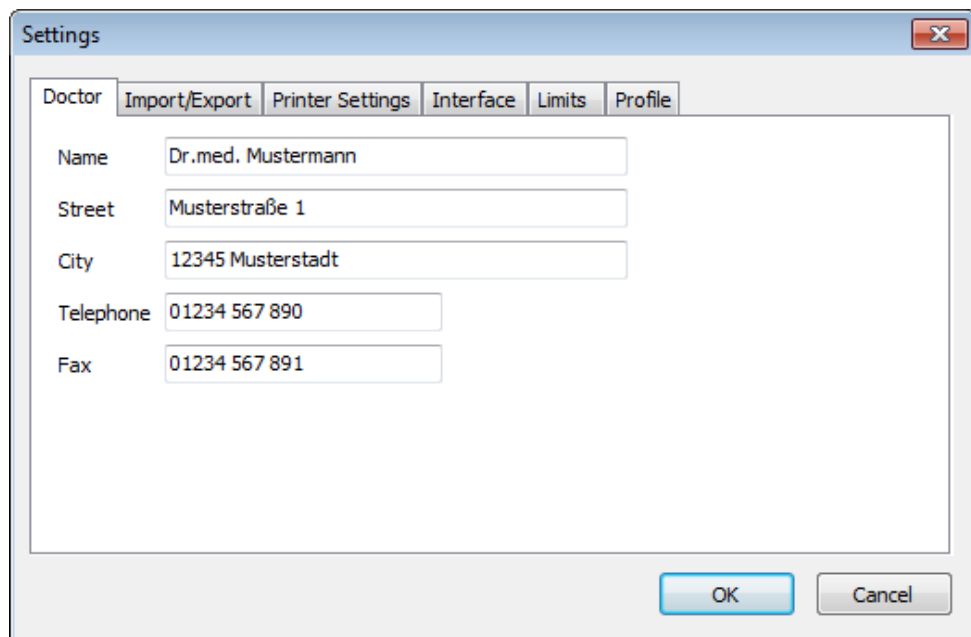


The screenshot shows a 'Settings' dialog box with a tabbed interface. The 'Doctor' tab is selected, showing fields for Name, Street, City, Telephone, and Fax. The other tabs are 'Import/Export', 'Printer Settings', 'Interface', 'Limits', and 'Profile'. The 'OK' and 'Cancel' buttons are at the bottom right.

Field	Value
Name	Dr.med. Mustermann
Street	Musterstraße 1
City	12345 Musterstadt
Telephone	01234 567 890
Fax	01234 567 891

The personal details of the doctor treating the patient are entered in the “Doctor” registry and used to produce the footer in the print-out.

4.7.2 "Import/Export" sub-registry

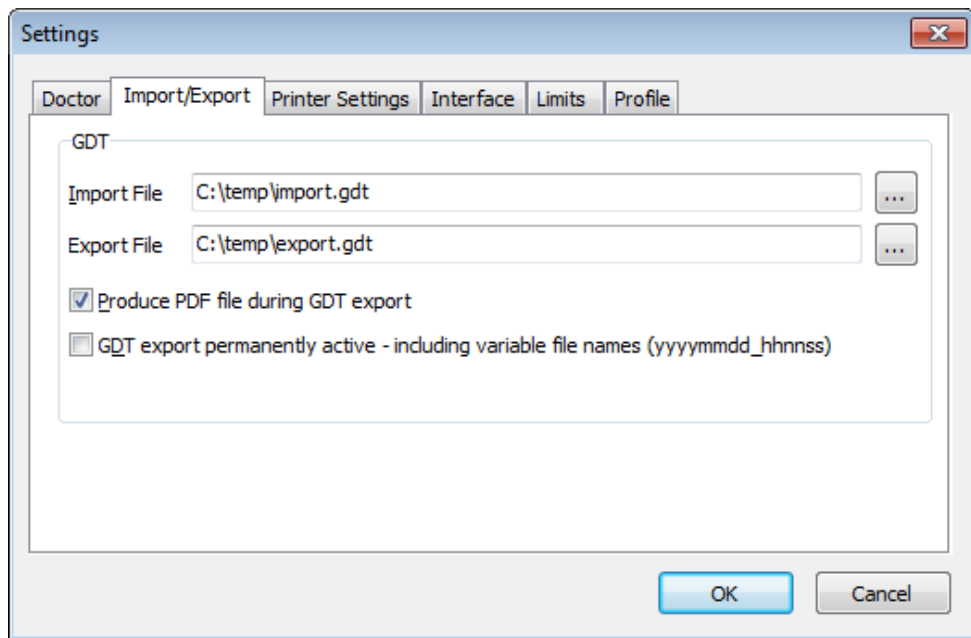

If you are using a clinic data processing system that supports the GDT interface, this is where the path and file names for export and import files are set. You have direct access to the Windows directory structure via the buttons next to the input fields for import and export files.

For example: c:\prax_ed\import.gdt
Import file = clinic DP system export file
Export file = clinic DP system import file

GDT import takes place automatically when you start the program, or manually by clicking the "Export/Import -> Import GDT" button if a valid GDT import file is present in the relevant directory.


GDT export takes place only if the patient being imported from the clinic DP system is active. Export takes place automatically when the program is closed down (if measurements have been read in from the device during the current program session) or can be performed manually at any time by clicking the "Export GDT" button in the "Measurements" registry.



Data export is deactivated if another patient has been selected after automatic import. It is reactivated when the first patient is reselected. Data export is also deactivated if no import has first taken place.

Further informations to the available options "Produce PDF file during GDT-export" and "GDT export permanently active" see 3.4.2 .

4.7.3 “Printer settings” sub-registry

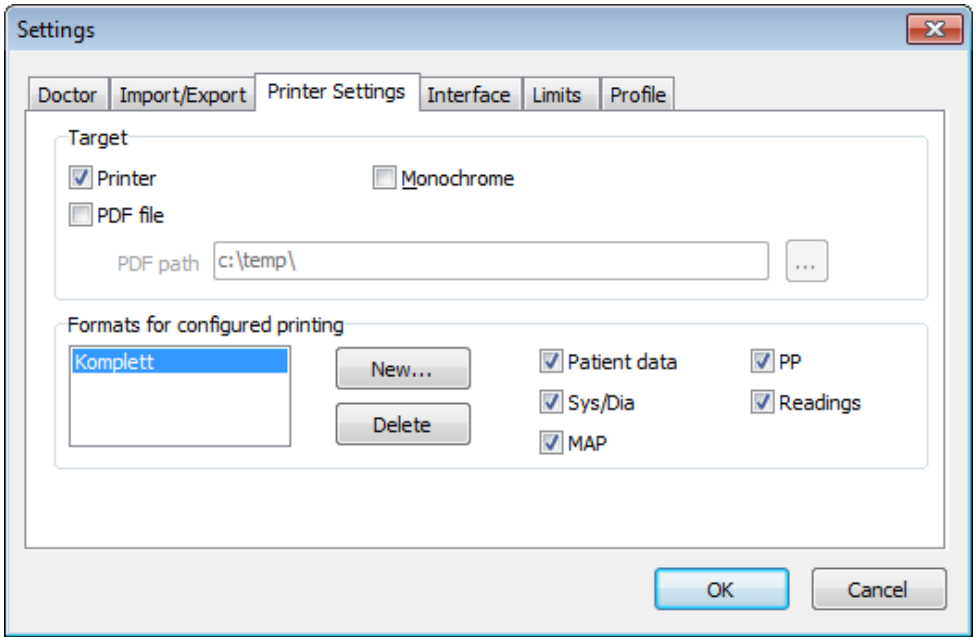

In the “Printer settings” registry you decide whether the print-out should be produced in paper form, as a screen print and/or as a PDF document, once the relevant [Print...] buttons have been clicked while the program is running.


If you select “Printer”, then the “Output Options” dialogue appears when you click on the [Print...] buttons while the program is running. You can choose either a print output (“Printer”) or a screen view (“Preview”). The “File” function has no significance here.

If you select “PDF file”, a PDF file is produced. The name of this PDF file is created in different ways depending on the application, and this process is described in more detail in the individual applications.




You must select at least one medium: “Printer” or “PDF file”.

If you select the “monochrome” option, the print will be in black and white. If you press the “Configured print-out” printer symbol, the print-out format configured here will be used and only the selected pages will be printed.

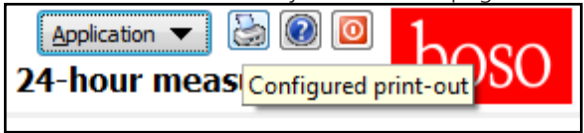

4.7.4 “Interface” sub-registry

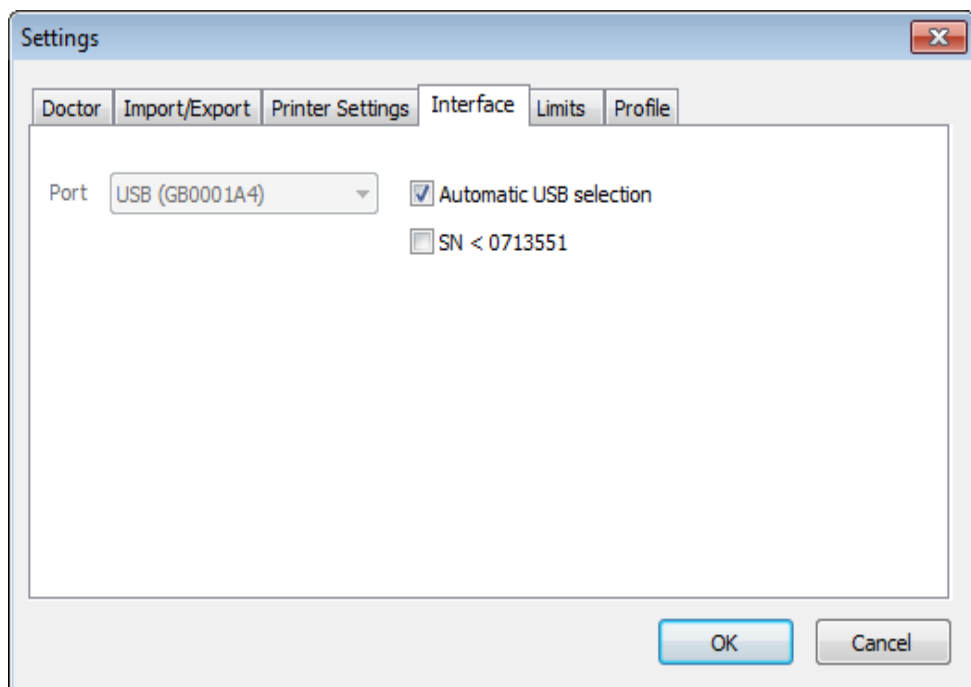

This is where you determine how the connection between the blood pressure meter TM-2430 and the PC is established.

If the “Automatic USB selection” is active, the software always checks which USB port a TM-2430 device is connected to before data transfer. If more than one device is connected at the same time, please disconnect all devices apart from the one that you want to use. You will see a warning telling you to do this.

If the “Automatic USB selection” option is not active, the serial (COM) or USB port selected in the port list will be used for data transfer.

Older models have a more limited set of instructions (no programmable patient number or maximum inflation pressure). Select the appropriate option for devices with serial numbers below SN M0713551.


4.7.5 “Limits” sub-registry

The screenshot shows a 'Settings' window with a tabbed interface. The 'Limits' tab is selected, showing three columns of input fields for 'Total', 'Day', and 'Night' periods. Each column contains five rows of physiological measurements: Systole, Diastole, Pulse, MAP, and PP. The 'Total' column has a blue border around its input fields. The 'Day' and 'Night' columns have grey borders. At the bottom right are 'OK' and 'Cancel' buttons.

Parameter	Total	Day	Night
Systole	130	135	120
Diastole	80	85	75
Pulse	100	110	90
MAP	100	110	90
PP	50	55	45

The limits for the individual periods can be set in order to allow customised assessment. The day and night limit settings relate to the interval periods that have been set.

4.7.6 “Profile” sub-registry

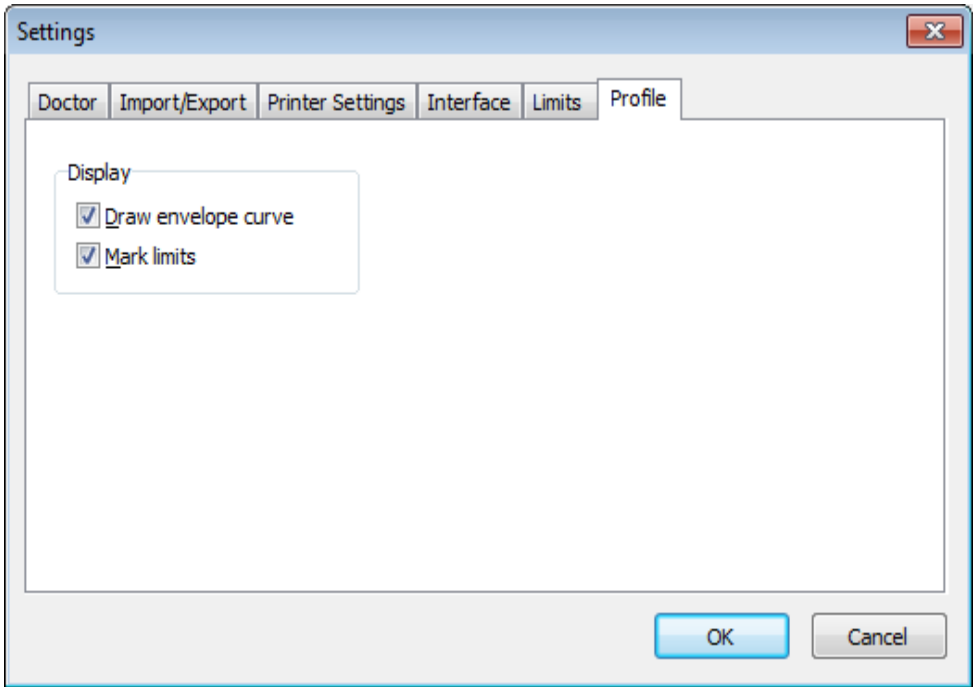

In the profile displays (“Sys/Dia, MAP, PP profile” registry), an envelope curve (line connecting the individual measurements) is normally drawn, with the limits shown as horizontal lines.

Both the envelope curve and the limit lines can be hidden.

5. "Patient measurement" application

5.1 "Patient" registry

see section "2.1 Patient registry, for all applications"

See chapter 4.7 for "Settings" button.

5.2 "Measurements" sub-registry

boso profilmanager XD




Name: **Mayer**

Forename: **Franz**


Patient no.: **10**

Birthdate: **04.11.1970**

Application



Patient measurement



Patient

Measurements

Sys/dia profile

MAP profile

PP profile

Statistics

Date	SYS	DIA	PUL	MAP	PP	Arr.	Exclude	Remark
1 Mo , 06.04.2005 - 18:26	144	75	65	98	69		<input type="checkbox"/>	Test
2 Do , 07.04.2005 - 08:32	159	88	68	112	71		<input type="checkbox"/>	
3 Do , 07.04.2005 - 18:37	153	92	67	112	61		<input type="checkbox"/>	
4 Fr , 08.04.2005 - 08:44	164	76	72	105	88		<input type="checkbox"/>	
5 Fr , 08.04.2005 - 18:49	152	87	68	109	65		<input type="checkbox"/>	
6 Sa , 09.04.2005 - 08:54	176	87	67	117	89		<input type="checkbox"/>	
7 Sa , 09.04.2005 - 18:59	160	99	67	119	61		<input type="checkbox"/>	
8 So , 10.04.2005 - 08:04	146	80	68	102	66		<input type="checkbox"/>	
9 So , 10.04.2005 - 18:09	153	82	66	106	71		<input type="checkbox"/>	
10 Mo , 11.04.2005 - 08:16	156	91	61	113	65		<input type="checkbox"/>	
11 Mo , 11.04.2005 - 18:20	160	84	65	109	76		<input type="checkbox"/>	
12 Di , 12.04.2005 - 08:28	151	88	60	109	63		<input type="checkbox"/>	
13 Di , 12.04.2005 - 18:34	152	81	64	105	71		<input type="checkbox"/>	
14 Mi , 13.04.2005 - 08:39	152	81	65	105	71		<input type="checkbox"/>	
15 Mi , 13.04.2005 - 18:46	177	86	62	116	91		<input type="checkbox"/>	
16 Do , 14.04.2005 - 08:51	161	89	60	113	72		<input type="checkbox"/>	
17 Do , 14.04.2005 - 18:57	163	86	70	112	77		<input type="checkbox"/>	
18 Fr , 15.04.2005 - 08:02	174	92	67	119	82		<input type="checkbox"/>	
19 Fr , 15.04.2005 - 18:07	166	96	71	119	70		<input type="checkbox"/>	
20 Sa , 16.04.2005 - 08:12	164	91	64	115	73		<input type="checkbox"/>	
21 Sa , 16.04.2005 - 18:17	148	91	70	110	57		<input type="checkbox"/>	
22 So , 17.04.2005 - 08:22	138	91	70	107	47		<input checked="" type="checkbox"/>	

Period

Device

06.04.2005 - 27.06.2005 medlife PC3

Delete Period...

Export GDT

Manual Data...

Print...

Transfer Data...

Interval limits...

☒ All

☐ Morning

☐ Afternoon

☐ Period

01.01.2012 - 31.12.2012

Version 4.1.0.108

User: sysdba

Server: localhost

Pattern: 41

DB: C:\Datenbanken\profman.fdb

All measurements that have been read in to date for the selected patient are displayed here. Both the period and the blood pressure meter with which the series of measurements was carried out are displayed.

	Date	SYS	DIA	PUL	MAP	PP	Arr.	Exclude	Remark
1	Mi, 06.04.2005 - 18:26	144	75	65	98	69		<input type="checkbox"/>	Test
2	Do, 07.04.2005 - 08:32	159	88	68	112	71		<input type="checkbox"/>	
3	Do, 07.04.2005 - 18:37	153	92	67	112	61		<input type="checkbox"/>	
4	Fr, 08.04.2005 - 08:44	164	76	72	105	88		<input type="checkbox"/>	
5	Fr, 08.04.2005 - 18:49	152	87	68	109	65		<input type="checkbox"/>	
6	Sa, 09.04.2005 - 08:54	176	87	67	117	89		<input type="checkbox"/>	
7	Sa, 09.04.2005 - 18:59	160	99	67	119	61		<input type="checkbox"/>	
8	So, 10.04.2005 - 08:04	146	80	68	102	66		<input type="checkbox"/>	
9	So, 10.04.2005 - 18:09	153	82	66	106	71		<input type="checkbox"/>	
10	Mo, 11.04.2005 - 08:16	156	91	61	113	65		<input type="checkbox"/>	
11	Mo, 11.04.2005 - 18:20	160	84	65	109	76		<input type="checkbox"/>	
12	Di, 12.04.2005 - 08:28	151	88	60	109	63		<input type="checkbox"/>	
13	Di, 12.04.2005 - 18:34	152	81	64	105	71		<input type="checkbox"/>	

The column content is as follows:

1: serial numbers of measurements

2: date and time of measurement

3: SYS = systolic blood pressure

4: DIA = diastolic blood pressure

5: PUL = pulse

6: MAP = mean arterial blood pressure, calculated as $DIA + 1/3 \text{ pulse pressure}$

7: PP = pulse pressure (SYS – DIA)

8: Arr. = indication of arrhythmia

9: Exclude = if you highlight this, the measurement will not be taken into account for assessment in the profile and statistics

10: Remark. Double-click in the measurement line to add a remark to a measurement.

This opens the remark input field:

Process remark

Date06.04.2005Time18:26

Sys144

Dia75

Puls65

MAP98

PP69

Remark

Test

OK

Cancel

5.2.1 “Delete period” button

This irrevocably deletes a complete set of readings.

5.2.2 “Export GDT” button

This generates the GDT export file manually. Only available if the GDT import of the active patient has already been performed.

5.2.3 “Manual data” button

Additional readings can be added to the active set of readings here.

5.2.4 “Print...” button

This prints out the list of readings.

If you selected “PDF file” in the printer settings (chapter 5.7.3), a PDF file will be created. The name of this PDF file is `medi_pat#_YYYYMMDD_m.pdf`

where


pat#=patient number

YYYYMMDD = date of measurement


m = measurement reference letter

5.2.5 “Transfer data” button


Connect the meter to the PC.

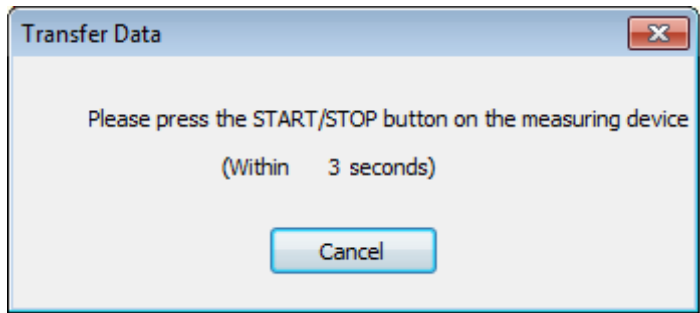

Once you have clicked on the “Transfer data” button, the START/STOP button on the blood pressure meter must be pressed within 6 seconds in order to transfer data from the blood pressure meter. Measurements will be transferred from the meter which is connected.

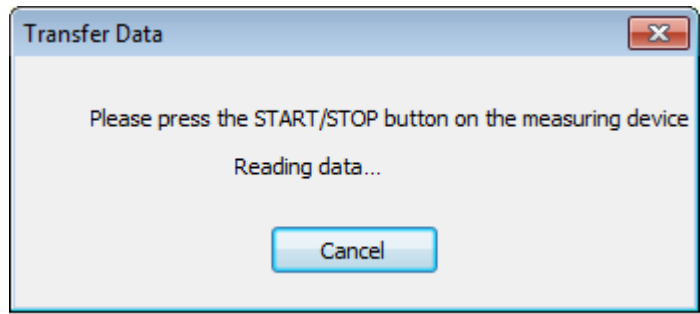

Once data has been successfully transferred, you can set up a new period or assign the data to an existing period.

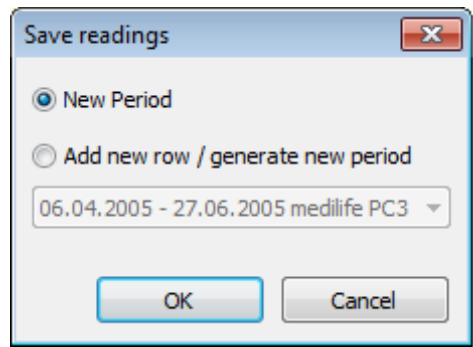

5.2.6 “Interval limits” button

The limits for morning and afternoon measurements can be defined here. The default setting is midnight to 11.59 a.m. for morning and noon to 11.59 p.m. for afternoon.

5.2.7 “All, Morning, Afternoon” selection

You can restrict the reading selection to only morning measurements or only afternoon measurements here.

5.2.8 “Period” selection

☒ Period 06.04.2005 - 10.02.2012

You can select a specific period for assessment among all the readings by selecting a period.

Click on the arrow symbol in the data fields to open a calendar, making selection easier.

Click on the month or year to change it immediately.


◀

Juni 2012

▶

Mo	Di	Mi	Do	Fr	Sa	So
28	29	30	31	1	2	3
4	5	6	7	8	9	10
11	12	13	14	15	16	17
18	19	20	21	22	23	24
25	26	27	28	29	30	1
2	3	4	5	6	7	8

5.3 “Sys/dia profile” registry

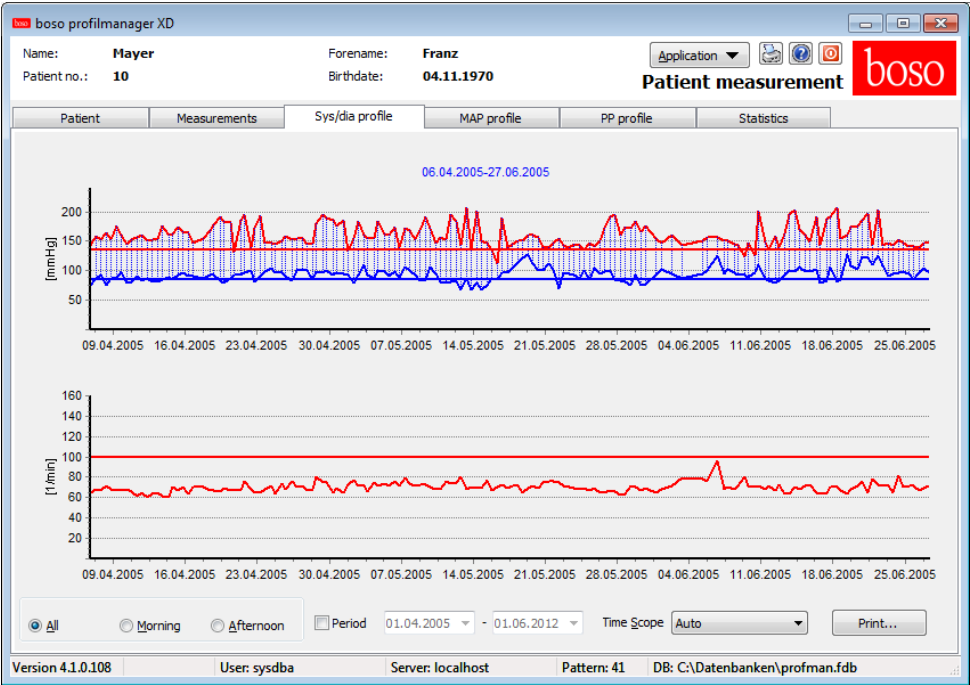

This displays the blood pressure trend.
The pulse trend can be hidden or displayed by the Ctrl+P key combination.

Move the cursor over the measurement to obtain more information about individual readings. The date, time and reading are displayed in the top left-hand corner of the diagram.

5.3.1 “All, Morning, Afternoon” selection

You can restrict the reading selection to only morning measurements or only afternoon measurements here.

5.3.2 “Period” selection

☒ Period

06.04.2005 ▾

-

10.02.2012 ▾

You can select a specific period for assessment among all the readings by selecting a period.

Click on the arrow symbol in the data fields to open a calendar, making selection easier.

Click on the month or year to change it immediately.

◀ Juni 2012 ▶						
Mo	Di	Mi	Do	Fr	Sa	So
28	29	30	31	1	2	3
4	5	6	7	8	9	10
11	12	13	14	15	16	17
18	19	20	21	22	23	24
25	26	27	28	29	30	1
2	3	4	5	6	7	8

5.3.3 “Time scope” selection field

This allows you to select the period for which measurements are displayed. You have the choice of Auto, Day, Week, Month, Quarter or Year.

“Auto” is the default setting. In this setting, the time scope is scaled from the first measurement to the last.


Right-clicking in the diagram allows you to shift the graph horizontally with the mouse.

5.3.4 “Print...” button

This produces a print-out of the SYS/DIA profile, pulse profile and statistics.
If you selected “PDF file” in the printer settings (chapter 5.7.3), a PDF file will be created.
The name of this PDF file is medi_pat#_YYYYMMDD_sys.pdf

where
pat#=patient number
YYYYMMDD = date of measurement
sys = SYS/DIA reference letter

5.4 “MAP profile” registry

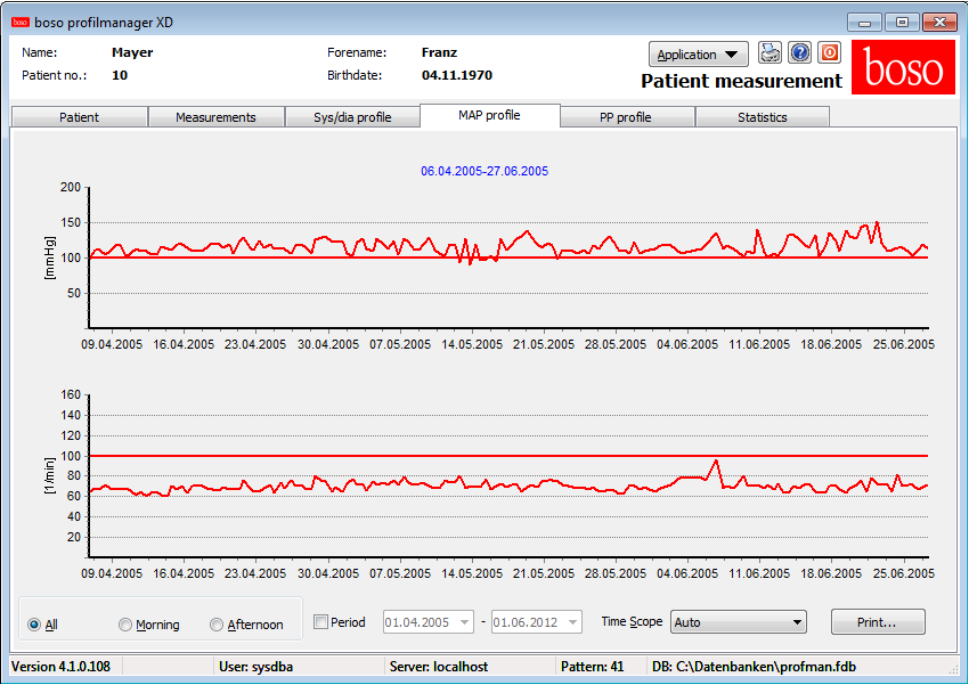

This displays the trend for the calculated mean arterial blood pressure. (MAP = diastole DIA + 1/3 pulse pressure PP).

The pulse trend can be hidden or displayed by the Ctrl+P key combination.

Move the cursor over the measurement to obtain more information about individual readings. The date, time and reading are displayed in the top left-hand corner of the diagram.

5.4.1 “All, Morning, Afternoon” selection

You can restrict the reading selection to only morning measurements or only afternoon measurements here.

5.4.2 “Period” selection

☒ Period 06.04.2005 - 10.02.2012

You can select a specific period for assessment among all the readings by selecting a period.

Click on the arrow symbol in the data fields to open a calendar, making selection easier.

Click on the month or year to change it immediately.



5.4.3 “Time scope” selection field

This allows you to select the period for which measurements are displayed. You have the choice of Auto, Day, Week, Month, Quarter or Year.

“Auto” is the default setting. In this setting, the time scope is scaled from the first measurement to the last.

Right-clicking in the diagram allows you to shift the graph horizontally with the mouse.


5.4.4 “Print...” button

This produces a print-out of the MAP profile, pulse profile and statistics.

If you selected “PDF file” in the printer settings (chapter 5.7.3), a PDF file will be created. The name of this PDF file is medi_pat#_YYYYMMDD_map.pdf

where
pat#=patient number
YYYYMMDD = date of measurement
map = MAP reference letter

5.5 “PP profile” registry

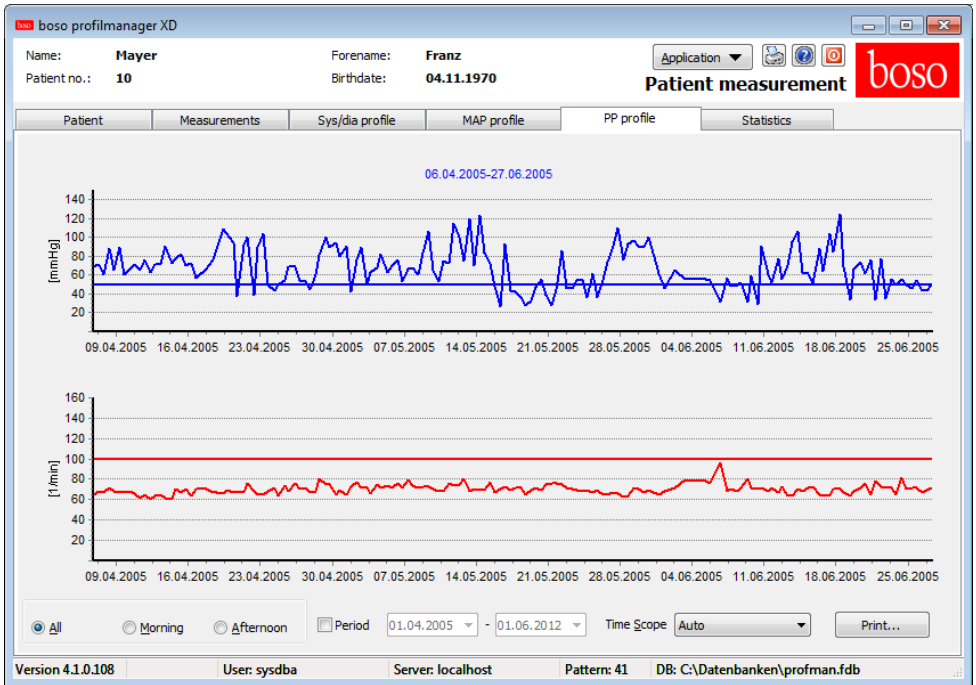

This displays the trend for the calculated pulse pressure. (PP = SYS-DIA).

The pulse trend can be hidden or displayed by the Ctrl+P key combination.

Move the cursor over the measurement to obtain more information about individual readings. The date, time and reading are displayed in the top left-hand corner of the diagram.

5.5.1 “All, Morning, Afternoon” selection

You can restrict the reading selection to only morning measurements or only afternoon measurements here.

5.5.2 “Period” selection

☒ Period

06.04.2005 ▾

-

10.02.2012 ▾

You can select a specific period for assessment among all the readings by selecting a period.

Click on the arrow symbol in the data fields to open a calendar, making selection easier.

Click on the month or year to change it immediately.

◀ Jun 2012 ▶						
Mo	Di	Mi	Do	Fr	Sa	So
28	29	30	31	1	2	3
4	5	6	7	8	9	10
11	12	13	14	15	16	17
18	19	20	21	22	23	24
25	26	27	28	29	30	1
2	3	4	5	6	7	8

5.5.3 “Time scope” selection field

This allows you to select the period for which measurements are displayed. You have the choice of Auto, Day, Week, Month, Quarter or Year.

“Auto” is the default setting. In this setting, the time scope is scaled from the first measurement to the last.

Right-clicking in the diagram allows you to shift the graph horizontally with the mouse.


5.5.4 “Print...” button

This produces a print-out of the pulse pressure profile, pulse profile and statistics.

If you selected “PDF file” in the printer settings (chapter 5.7.3), a PDF file will be created. The name of this PDF file is medi_pat#_YYYYMMDD_pp.pdf

where
pat#=patient number
YYYYMMDD = date of measurement
pp = pulse pressure reference letter

5.6 “Statistics” registry

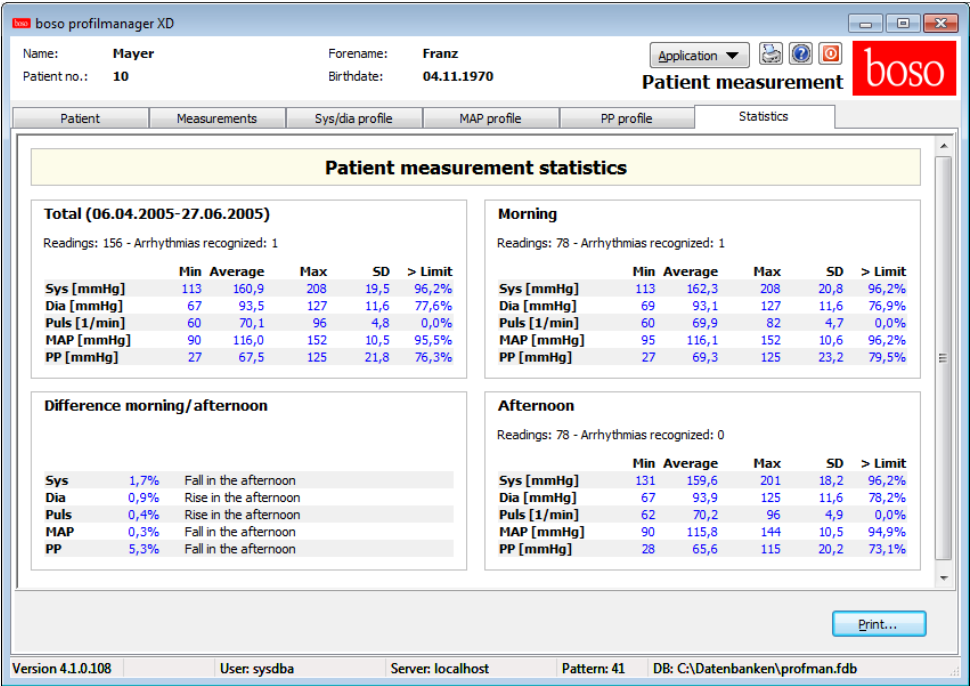

Measurements for the complete period, morning and afternoon periods are assessed separately.

The total number of readings in the individual periods, and the number of arrhythmias recognised, are displayed.

The following values are displayed in the individual columns:

Min: smallest value in the interval in question

Mean: arithmetic mean in the interval in question

Max: largest value in the interval in question

SD: standard deviation in the interval in question

> Limit: percentage above the limits that have been set

The percentage increase/decrease in the afternoon is displayed.

5.6.1 “Print...” button

This produces a print-out of the SYS/DIA profile, pulse profile and statistics.

If you selected “PDF file” in the printer settings (chapter 5.7.3), a PDF file will be created. The name of this PDF file is `medi_pat#_YYYYMMDD_sys.pdf`

where


pat#=patient number

YYYYMMDD = date of measurement

sys = SYS/DIA reference letter

5.7 “Settings...” button in “Patient” registry

5.7.1 “Doctor” sub-registry

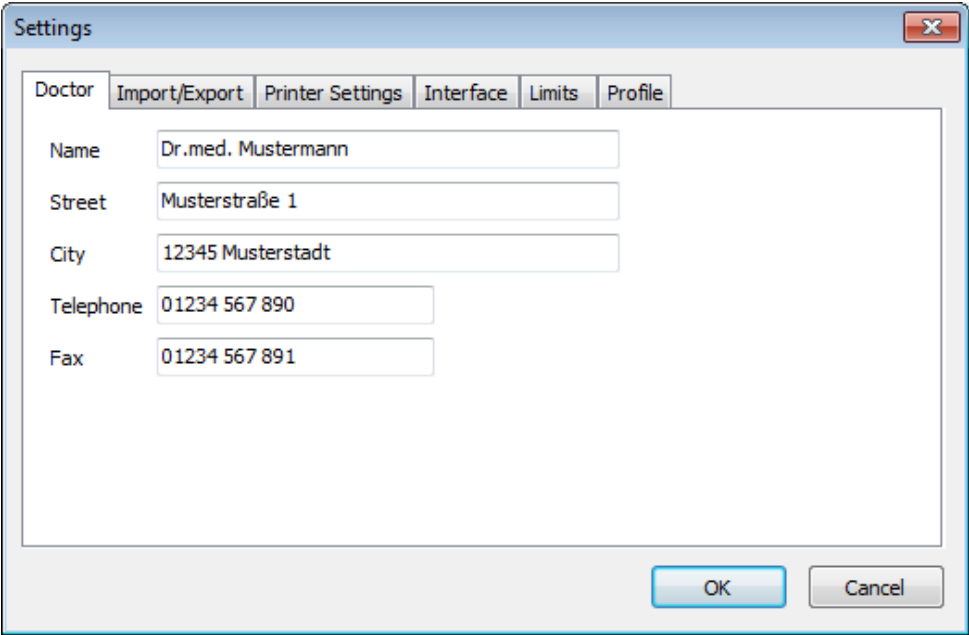


The screenshot shows a 'Settings' dialog box with a tabbed interface. The 'Doctor' tab is selected, showing input fields for Name, Street, City, Telephone, and Fax. The other tabs are 'Import/Export', 'Printer Settings', 'Interface', 'Limits', and 'Profile'. The 'OK' and 'Cancel' buttons are at the bottom right.

Field	Value
Name	Dr.med. Mustermann
Street	Musterstraße 1
City	12345 Musterstadt
Telephone	01234 567 890
Fax	01234 567 891

The personal details of the doctor treating the patient are entered in the “Doctor” registry and used to produce the footer in the print-out.

5.7.2 "Import/Export" sub-registry

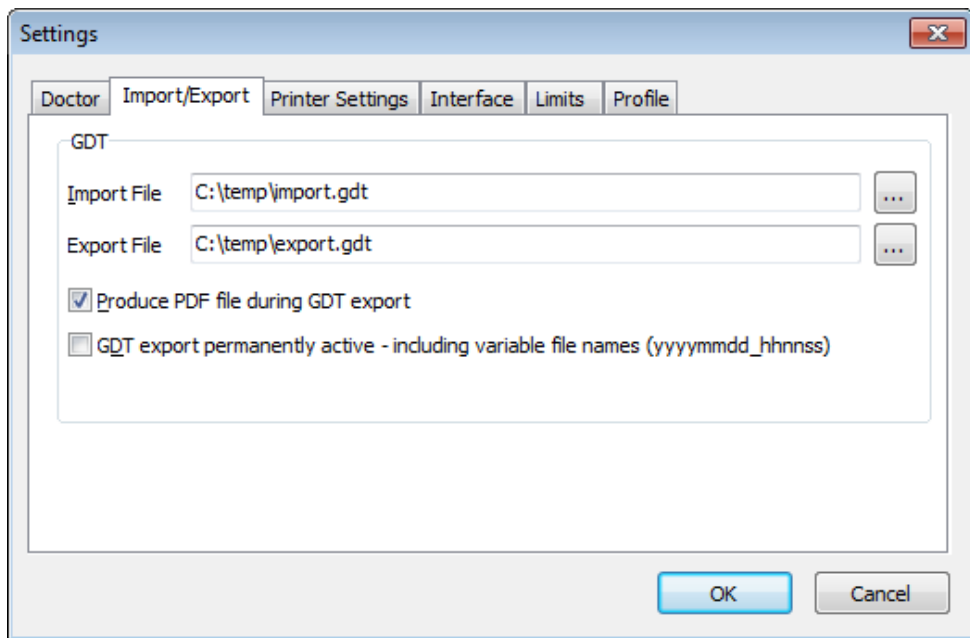

If you are using a clinic data processing system that supports the GDT interface, this is where the path and file names for export and import files are set. You have direct access to the Windows directory structure via the buttons next to the input fields for import and export files.

For example: c:\prax_ed\import.gdt
Import file = clinic DP system export file
Export file = clinic DP system import file

GDT import takes place automatically when you start the program, or manually by clicking the "Export/Import -> Import GDT" button if a valid GDT import file is present in the relevant directory.


GDT export takes place only if the patient being imported from the clinic DP system is active. Export takes place automatically when the program is closed down (if measurements have been read in from the device during the current program session) or can be performed manually at any time by clicking the "Export GDT" button in the "Measurements" registry.



Data export is deactivated if another patient has been selected after automatic import. It is reactivated when the first patient is reselected. Data export is also deactivated if no import has first taken place.

Further informations to the available options "Produce PDF file during GDT-export" and "GDT export permanently active" see 3.4.2 .

5.7.3 “Printer settings” sub-registry

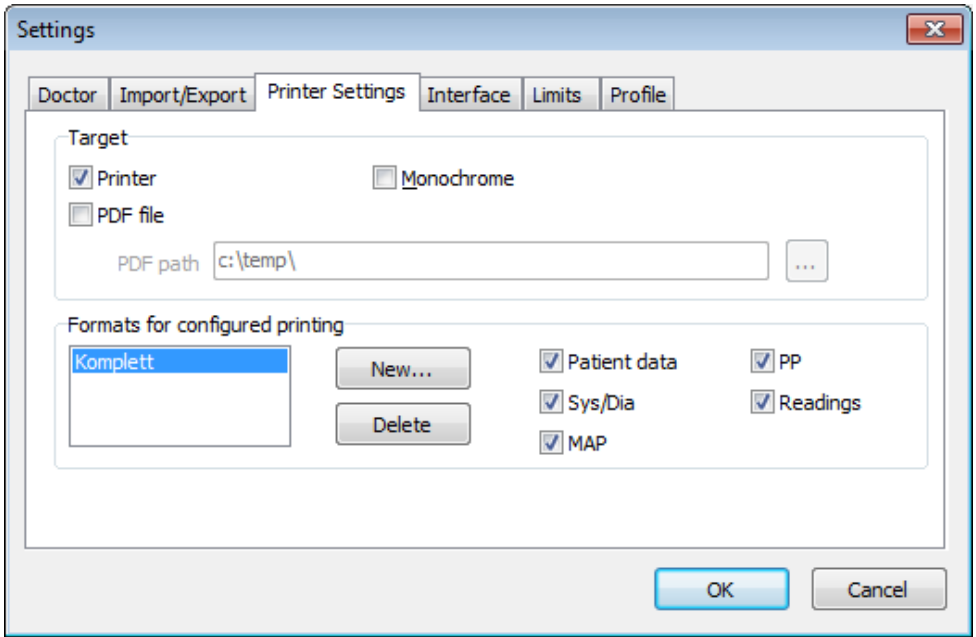

In the “Printer settings” registry you decide whether the print-out should be produced in paper form, as a screen print and/or as a PDF document, once the relevant [Print...] buttons have been clicked while the program is running.


If you select “Printer”, then the “Output Options” dialogue appears when you click on the [Print...] buttons while the program is running. You can choose either a print output (“Printer”) or a screen view (“Preview”). The “File” function has no significance here.

If you select “PDF file”, a PDF file is produced. The name of this PDF file is created in different ways depending on the application, and this process is described in more detail in the individual applications.




You must select at least one medium: “Printer” or “PDF file”.

If you select the “monochrome” option, the print will be in black and white.
If you press the “Configured print-out” printer symbol, the print-out format configured here will be used and only the selected pages will be printed.



5.7.4 “Interface” sub-registry

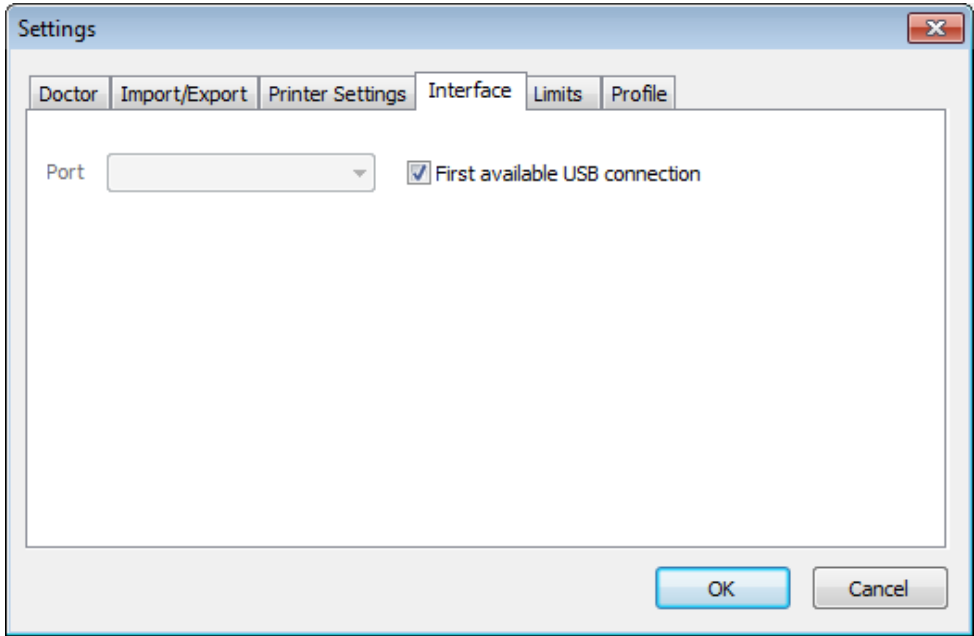

If the “First available USB port” option is active, the first FTDI USB port under Windows will be used to transfer data. If more than one FTDI USB port is installed, disconnect the ports that are not needed from the computer, or deactivate the option.

If the “First available USB port” option is not active, the serial (COM) interface or USB port selected in the port list will be used for data transfer.

5.7.5 “Limits” sub-registry

Settings


DoctorImport/ExportPrinter SettingsInterfaceLimitsProfile

Total	Day	Night
Systole130	Systole135	Systole120
Diastole80	Diastole85	Diastole75
Pulse100	Pulse110	Pulse90
MAP100	MAP110	MAP90
PP50	PP55	PP45

OKCancel

The limits for the individual periods can be set in order to allow customised assessment. The limit settings for morning and afternoon are based on the morning and afternoon interval periods.

5.7.6 “Profile” sub-registry

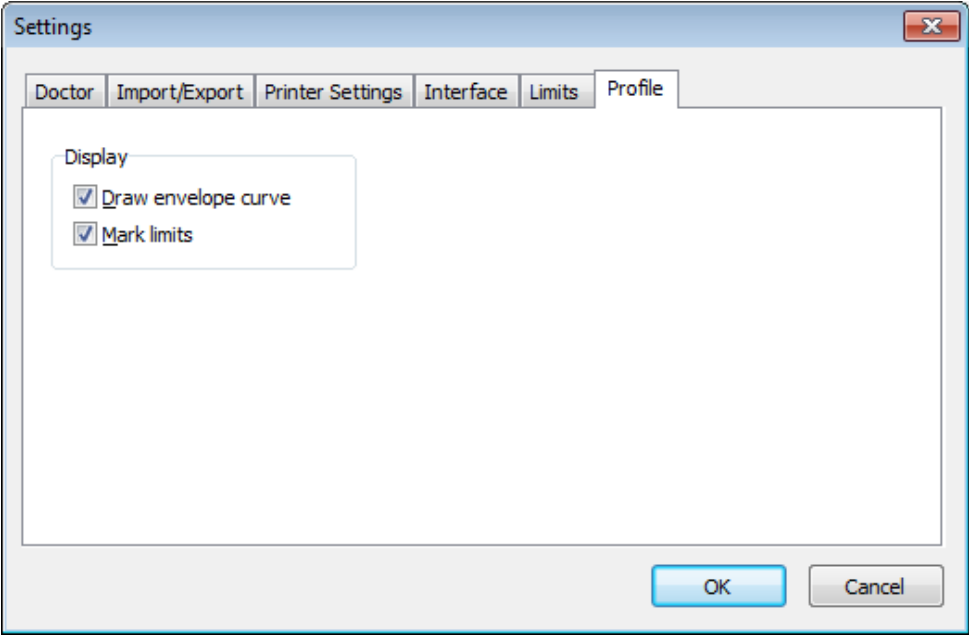

In the profile displays (“Sys/Dia, MAP, PP profile” registry), an envelope curve (line connecting the individual measurements) is normally drawn, with the limits shown as a horizontal line.

Both the envelope curve and the limit lines can be hidden.

6. Warranty provisions

Irrespective of statutory warranty rights, boso guarantees the software data carrier to be free from material and processing defects for 90 days from the date of purchase.

In the light of the warranty undertaking given above, boso is obliged to replace the data carrier and the software it contains under the following conditions:

- the customer/purchaser notifies boso of the defect in writing within 90 days of the date of purchase

or

- the customer/purchaser returns the defective data carrier to the dealer, or direct to boso at the address below, within 90 days:

boso
BOSCH + SOHN GmbH u. Co. KG
Bahnhofstr. 64
D-72417 Jungingen
Germany

boso does not offer any warranty, either explicitly or tacitly, beyond the warranty undertaking given above.

7. Limitation of liability

- a) The software is supplied to you on the basis of the current state of development.
- b) Irrespective of the provision set out in chapter 6, boson and its dealers accept no liability for risks with regard to the results and performance of the software. We bear no liability for indirect losses, consequential losses, loss of earnings, losses due to lost or damaged data or other commercial or financial losses.
- c) The aforementioned exclusion of liability does not apply to liability under product liability legislation or to cases of deliberate action or gross negligence on our part or on the part of our agents.

8. Explanation of symbols



Read the user instructions



Year of manufacture



Manufacturer



The CE mark documents compliance with the Medical Devices Directive 93/42/EEC,
Notified body: DEKRA, 0124



Important notice

Appendix A - Extract from GDT record description

The record types and their field identifiers needed to create the GDT interface of this software are described below:

Record type 6302 "Request new examination"

Field 8000: record identification

8100: record length

8315: GDT ID of recipient

8316: GDT ID of sender

8410: Testident (BDM00: shortcut patient measurement

BDM01: shortcut 24-hour measurement

BDM02: shortcut ABI/PWV measurement)

9218: GDT version number

3000: patient number

3101: patient's surname

3102: patient's first name

3103: patient's date of birth

3105: insurance number

3106: patient's address (town)

3107: patient's address (street)

3110: patient's gender (1 = male, 2 = female)

3622: patient's height (cm)

3623: patient's weight (kg)

Record type 6310 "Transmit data from examination"

Field 8000: record identification

8100: record length

8315: GDT ID of recipient

8316: GDT ID of sender

9218: GDT version number

3000: patient number / patient identification

8402: Map for a particular device and process

6200: Date of examination

6228: Results table text, formatted

6302: File archiving identifier

6303: File format

6304: File content

6305: File reference

 **BOSCH + SOHN GmbH u. Co. KG**
Bahnhofstraße 64 • 72417 Jungingen • Germany
Phone: +49 (0) 74 77 / 92 75-0 • Telefax: +49 (0) 74 77 / 10 21
www.boso.de • mail: zentrale@boso.de